

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED

JUN 20 2016

FDLE

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Alcohol Testing Program

Agency: ORANGE COUNTY SO
Time of Inspection: 06:47

Date of Inspection: 06/17/2016

Serial Number: 80-000964
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____


Number of Simulators Used: _____

Remarks:

BYPASS TO OPERATE INSTRUMENT Non-compliance: NOT YET DETERMINED.

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

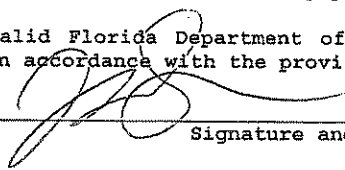

JAKE L SHANAHAN

Signature and Printed Name

06/17/2016
Date

ORANGE COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000964
06/17/2016
Software: 8100.27

INTOXILYZER 8000
Instrument Initialization
06:21 06/17/2016

ORANGE COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000964
06/17/2016
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:52
Control Test	0.049	06:53
Air Blank	0.000	06:53
Control Test	0.049	06:54
Air Blank	0.000	06:54
Control Test	0.050	06:55
Air Blank	0.000	06:56
Control Test Stats		
Average	0.0493	
Std Dev	0.0006	
Rel Std Dev(%)	1.1703	

Test	g/210L	Time
Air Blank	0.000	06:48
Control Test	0.079	06:48
Air Blank	0.000	06:49
Control Test	0.079	06:49
Air Blank	0.000	06:50
Control Test	0.079	06:50
Air Blank	0.000	06:51
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

DGS

Operator's Signature

ORANGE COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000964
06/17/2016
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	06:57
Control Test	0.195	06:57
Air Blank	0.000	06:58
Control Test	0.198	06:58
Air Blank	0.000	06:59
Control Test	0.199	07:00
Air Blank	0.000	07:00
Control Test Stats		
Average	0.1973	
Std Dev	0.0021	
Rel Std Dev(%)	1.0549	

Operator's Signature

Operator's Signature

Operator's Signature

Test	g/210L	Time
Air Blank	0.000	07:01
Control Test	0.078	07:02
Air Blank	0.000	07:02
Control Test	0.079	07:03
Air Blank	0.000	07:03
Control Test	0.079	07:04
Air Blank	0.000	07:05
Control Test Stats		
Average	0.0787	
Std Dev	0.0006	
Rel Std Dev(%)	0.7339	

ORANGE COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-000964
06/17/2016
Software: 8100.27