

998 ~~9~~ RECEIVED

Florida Department of Law Enforcement Alcohol Testing Program

NOV 02 2016

FDLE
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: SEMINOLE COUNTY S.O.
Time of Inspection: 02:53

Date of Inspection: 10/29/2016

Serial Number: 80-000998
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1789170 Exp: 01/14/2018
0.000	0.047	0.078	0.196	0.081
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.077	0.198	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

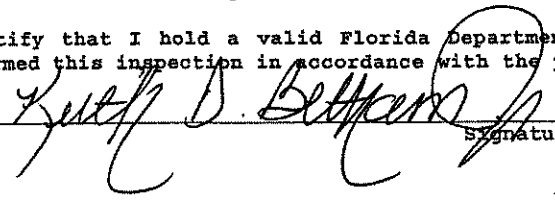

KEITH D BETHAM

Signature and Printed Name

10/29/2016
Date