

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
DEC 29 2016  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 22:31

Date of Inspection: 12/28/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:477627 Exp: 06/29/2019
0.000	0.049	0.077	0.196	0.079
0.000	0.049	0.078	0.197	0.079
0.000	0.050	0.079	0.197	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
\_\_\_\_\_  
Signature and Printed Name

JOSHUA C CAMPBELL

12/28/2016  
Date

RECEIVED  
11/29/2016

# Florida Department of Law Enforcement Alcohol Testing Program

FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 21:40

Date of Inspection: 11/29/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#: 201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#: 201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 477627 Exp: 06/29/2019
0.000	0.048	0.079	0.198	0.078
0.000	0.049	0.079	0.199	0.079
0.000	0.048	0.080	0.199	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JOSHUA C CAMPBELL

Signature and Printed Name

11/29/2016  
Date

RECEIVED

OCT 26 2016

Florida Department of Law Enforcement  
Alcohol Testing Program

00

FDLE

Alcohol

Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 21:38

Date of Inspection: 10/26/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.048	0.079	0.195	0.077
0.000	0.048	0.079	0.195	0.077
0.000	0.048	0.079	0.195	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JOSHUA C CAMPBELL

Signature and Printed Name

10/26/2016  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
SEP 28 2016  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 22:08

Date of Inspection: 09/28/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	



Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.048	0.078	0.194	0.077
0.000	0.048	0.078	0.196	0.076
0.000	0.048	0.078	0.197	0.076

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



 JOSHUA C CAMPBELL *A. Hernandez*  
 Signature and Printed Name

09/28/2016  
Date

RECEIVED  
AUG 02 2016  
FDLE  
Alcohol Testing Program

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:38

Date of Inspection: 08/02/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	



Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.047	0.078	0.195	0.077
0.000	0.047	0.078	0.198	0.077
0.000	0.048	0.078	0.198	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  JOSHUA C CAMPBELL / Alain Hernandez  
Signature and Printed Name

08/02/2016  
Date

80-003411 (10)

RECEIVED

MAY 22 2016

# Florida Department of Law Enforcement Alcohol Testing Program

FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 22:28

Date of Inspection: 05/22/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.048	0.076	0.198	0.079
0.000	0.048	0.076	0.200	0.080
0.000	0.049	0.077	0.200	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JOSHUA C CAMPBELL  
Signature and Printed Name

05/22/2016  
Date

RECEIVED

APR 28 2016

FDLE  
Alcohol Testing Program

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:44

Date of Inspection: 04/28/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.046	0.075	0.196	0.080
0.000	0.047	0.076	0.197	0.080
0.000	0.047	0.076	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

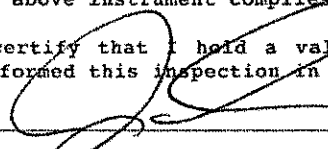

JOSHUA C CAMPBELL

Signature and Printed Name

04/28/2016  
Date

RECEIVED

# Florida Department of Law Enforcement Alcohol Testing Program

MAR 29 2016

FDLE

Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 22:57

Date of Inspection: 03/28/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.049	0.077	0.197	0.080
0.000	0.049	0.078	0.197	0.080
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JOSHUA C CAMPBELL

Signature and Printed Name

03/28/2016  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**

FEB 25 2016

FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:18

Date of Inspection: 02/24/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201411K Exp: 11/25/2016	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:28814080A3 Exp: 11/05/2016
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.079	0.199	0.080
0.000	0.049	0.079	0.197	0.080

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JOSHUA C CAMPBELL

Signature and Printed Name

02/24/2016  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
**FEB 25 2016**  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 22:15

Date of Inspection: 01/15/2016

Serial Number: 80-003411  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201411K Exp: 11/25/2016	0.08g/210L Test (g/210L) Lot#: 201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#: 201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 2881408CA3 Exp: 11/05/2016
0.000	0.046	0.076	0.196	0.080
0.000	0.046	0.076	0.196	0.080
0.000	0.047	0.077	0.195	0.080

Number of Simulators Used: 4

Remarks:  
JAN INSPECTION

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

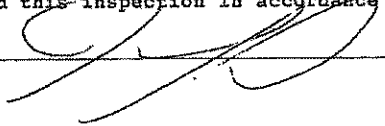

JOSEPH S ANGELICCHI

Signature and Printed Name

01/15/2016  
Date