

Florida Department of Law Enforcement
 Alcohol Testing Program

JUN 28 2016

FDLE
 Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
 Time of Inspection: 15:41

Date of Inspection: 06/23/2016

Serial Number: 80-003935
 Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1578837 Exp: 10/16/2016
0.000	0.047	0.075	0.198	0.079
0.000	0.048	0.077	0.199	0.079
0.000	0.048	0.078	0.198	0.079


Number of Simulators Used: 5

Remarks:

gdm

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

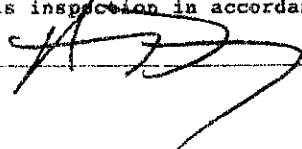

Signature and Printed Name ANGEL M DIAZ

06/23/2016
 Date

Florida Department of Law Enforcement
 Alcohol Testing Program

JUN 28 2016

FDLE
 Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
 Time of Inspection: 15:41

Date of Inspection: 06/23/2016

Serial Number: 80-003935
 Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#: 201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#: 201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 1578837 Exp: 10/16/2016
0.000	0.047	0.075	0.198	0.079
0.000	0.048	0.077	0.199	0.079
0.000	0.048	0.078	0.198	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

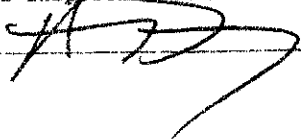

ANGEL M DIAZ

Signature and Printed Name

06/23/2016
 Date