

# Florida Department of Law Enforcement

## Alcohol Testing Program *PJM*

RECEIVED *✓ 2/5/16*

JAN 06 2016

FDLE

### DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000 *Alcohol Testing Program*

Agency: MARION COUNTY SO  
Time of Inspection: 11:04

Date of Inspection: 01/06/2016

Serial Number: 80-000827  
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

BK

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201502G Exp: 02/24/2017	0.20g/210L Test (g/210L) Lot#:201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG511701 Exp: 04/27/2017
0.000	0.052	0.082	0.204	0.081
0.000	0.052	0.083	0.206	0.081
0.000	0.052	0.082	0.207	0.080
0.000	0.052	0.082	0.206	0.080
0.000	0.053	0.083	0.207	0.081
0.000	0.052	0.082	0.207	0.080
0.000	0.053	0.083	0.206	0.080
0.000	0.053	0.083	0.206	0.080
0.000	0.053	0.083	0.206	0.080
0.000	0.053	0.083	0.206	0.080
0.000	0.052	0.083	0.206	0.080

Standard Deviations	0.0005	0.0005	0.0008	0.0004
---------------------	--------	--------	--------	--------


Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0005 Number of Simulators Used: 5

**Remarks:**

A F / M A: SAMPLE NOT LONG ENOUGH

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

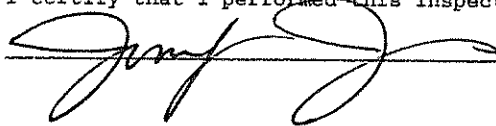

JENNIFER H JACOBS  
Signature and Printed Name

01/06/2016  
Date