

RECEIVED

Bec

SEP 07 2016

FDLE

Alcohol Testing Program

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: ALTAMONTE SPRINGS PD
Time of Inspection: 12:29

Date of Inspection: 09/07/2016

Serial Number: 80-000997
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG612405 Exp: 05/03/2018
0.000	0.050	0.080	0.198	0.000 / 0.079
0.000	0.050	0.081	0.199	0.079 / 0.079
0.000	0.050	0.081	0.199	0.078 / 0.079
0.000	0.051	0.081	0.199	0.079 / 0.079
0.000	0.050	0.081	0.198	0.079 / 0.079
0.000	0.050	0.081	0.198	0.079 / 0.079
0.000	0.050	0.081	0.198	0.078 / 0.079
0.000	0.050	0.081	0.198	0.078 / 0.079
0.000	0.050	0.081	0.199	0.078 / 0.079
0.000	0.050	0.080	0.198	0.078 / 0.079

Standard Deviations	0.0003	0.0004	0.0005	0.0248 / 0.0000
---------------------	--------	--------	--------	-----------------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance DGS NOT CONNECTED FIRST RUN .

*MWS
BK*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

JAKE L SHANAHAN

Signature and Printed Name

09/07/2016
Date

RECEIVED

bes

SEP 07 2016

Florida Department of Law Enforcement Alcohol Testing Program

FDLE

Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: ALTAMONTE SPRINGS PD
Time of Inspection: 12:29

Date of Inspection: 09/07/2016

Serial Number: 80-000997
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG612405 Exp: 05/03/2018
0.000	0.050	0.080	0.198	0.000 / 0.079
0.000	0.050	0.081	0.199	0.079 / 0.079
0.000	0.050	0.081	0.199	0.078 / 0.079
0.000	0.051	0.081	0.199	0.079 / 0.079
0.000	0.050	0.081	0.198	0.079 / 0.079
0.000	0.050	0.081	0.198	0.079 / 0.079
0.000	0.050	0.081	0.198	0.078 / 0.079
0.000	0.050	0.081	0.198	0.078 / 0.079
0.000	0.050	0.081	0.199	0.078 / 0.079
0.000	0.050	0.080	0.198	0.078 / 0.079

Standard Deviations	0.0003	0.0004	0.0005	0.0248 / 0.0000
---------------------	--------	--------	--------	-----------------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5


Remarks:

08: Control Outside Tolerance DGS NOT CONNECTED FIRST RUN .

*PWS
ASK*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

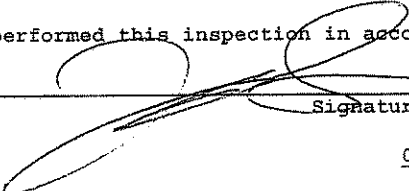

Signature and Printed Name

JAKE L SHANAHAN

09/07/2016
Date