

Florida Department of Law Enforcement

Alcohol Testing Program

RECEIVED *✓/500*

SEP 13 2016

FDLE

Alcohol Testing Program *6/6*

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 08:27

Date of Inspection: 09/12/2016

Serial Number: 80-003410
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK		No	Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK		No	Barometric Pressure Sensor Check: OK		No
Alcohol Free Subject Test: 0.000		No	Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No	Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

ADM

Standard Deviations			
---------------------	--	--	--


Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: _____ Number of Simulators Used: _____

Remarks:
TIME INCORRECT

Corrected & Retest.

(Signature)

The above instrument complies () does not comply () with Chapter 11D-8, FAC.
I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

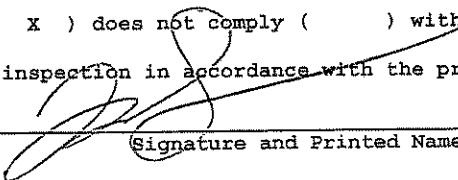

 Signature and Printed Name

09/12/2016
Date

RECEIVED

Florida Department of Law Enforcement Alcohol Testing Program

SEP 13 2016

FDLE

Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 11:08

Date of Inspection: 09/12/2016

Serial Number: 80-003410
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201507 Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG612405 Exp: 05/03/2018
0.000	0.050	0.080	0.198	0.080
0.000	0.050	0.080	0.198	0.080
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.081	0.198	0.079
0.000	0.050	0.080	0.199	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.080	0.198	0.079
0.000	0.050	0.080	0.198	0.079


Standard Deviations	0.0000	0.0003	0.0003	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0002 Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

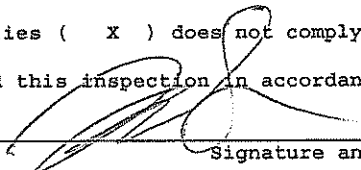

JAKE L SHANAHAN

Signature and Printed Name

09/12/2016
Date