

INSTRUMENT PROCESSING SHEET

Agency Broward County Sheriff's Office S/N 80-006475
 Date In 8/25/2016 Date Out 8/25/2016 Ship P/U H/D CMI EE

Intake Performed By DELL

Registration
 Annual
 Return from CMI
 Return from Enforcement
 Electronics
 Other _____

Visual Inspection:
OK Case OK Handle
OK Dry Gas Holder OK Feet
OK Keyboard/Plug OK Back/Plugs
OK Screws tight OK Breath Hose

Other Equipment:
 Power cord
 Printer Cable
 Other _____

Notes: _____

Quality Checks Performed By DELL

Breath Tube Screen
 Replace O-Rings
 Instrument Set Up Verified
 R-Value 172
 Flow Verification (L/s)
 Flow Column # ATP 101
 32mm 156 (.139 - .169)
 36mm 175 (.156 - .190)
 53mm 242 (.228 - .278)
 103mm 500 (.447 - .547)

Barometric Pressure Check
 Gauge ID # 28663

Stability Checks

Simulator	Serial #	Lot #/Exp
0.05	SD3967	201507A 07/14/2017
0.08	SD3968	201601F 01/26/2018
0.20	SD3969	201505A 05/12/2017
0.08 DGS	N/A	AG600504 01/05/2018

Flow Calibration Performed By DELL

Flow Calibration N/A
 Flow Calibration Complete
 Flow Column # _____
 5L/min - 17mm
 15L/min - 53mm
 30L/min - 103mm

R-Value _____
 Post Calibration Verification (L/s)
 Flow Column # _____
 32mm _____ (.139 - .169)
 36mm _____ (.156 - .190)
 53mm _____ (.228 - .278)
 103mm _____ (.447 - .547)

Maintenance Performed By _____

Battery Replacement
 Dry Gas Regulator Replacement
 Breath Tube Replacement
 Other _____

Suggested Service

RECEIVED
 SEP 07 2016
 FDLE
 Alcohol Testing Program

Optical Bench Calibration Performed By _____

Optical Bench Calibration N/A
 Optical Bench Calibration Complete

Barometric Pressure Gauge ID # _____

Simulator	Serial Number	Lot Number	Expiration
0.000		N/A	N/A
0.040			
0.100			
0.200			
0.400			
0.080 DGS	N/A		

Post Calibration Stability Checks

Simulator	Serial Number	Lot Number	Expiration
0.05			
0.08			
0.20			
0.08 DGS	N/A		

Department Inspection Performed By DELL

Barometric Pressure 1014 Gauge
 ID# 28199 1014 Instrument

Mouth Alcohol Solution Lot # 2016-A
 Acetone Stock Solution Lot # 2016-B

Simulator	Serial Number
0.00	SD 3965
Interferent	SD 3964
0.05	SD 3967
0.08	SD 3968
0.20	SD 3969

Attachments

Form 41
 Pre-Stability Tests
 Flow Calibration

Optical Bench Cal
 Post-Stability Tests
 Other _____

Notes: **E-MAILED** **APPROVED**
08/25/2016
PA/OC OK 9/6/16
Brett Kirkland
 Quality Control Review

Instrument Complies with Chapter 11D-8, FAC
 Instrument Does Not Comply with Chapter 11D-8, FAC
 Return to/Place into Evidentiary Use
 Remain Out of Evidentiary Use
 Conduct an Agency Inspection Before Evidentiary Use

9/7/16
 Date

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities	80-006475	Broward County Sheriff's Office	08/25/2016	<i>[Signature]</i>

[Handwritten initials]

0.05g/210L	0.08g/210L	0.20g/210L	DGS 0.08g/210L
0.047 to 0.053 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>	0.194 to 0.206 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>

BROWARD COUNTY SO
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006475
 08/25/2016
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:24
Control Test	0.048	11:24
Air Blank	0.000	11:25
Control Test	0.049	11:25
Air Blank	0.000	11:26
Control Test	0.049	11:27
Air Blank	0.000	11:27

Control Test Stats
 Average 0.0487
 Std Dev 0.0006
 Rel Std Dev(%) 1.1863

[Signature]
 Operator's Signature

BROWARD COUNTY SO
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006475
 08/25/2016
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:29
Control Test	0.078	11:29
Air Blank	0.000	11:30
Control Test	0.079	11:31
Air Blank	0.000	11:31
Control Test	0.079	11:32
Air Blank	0.000	11:32

Control Test Stats
 Average 0.0787
 Std Dev 0.0006
 Rel Std Dev(%) 0.7339

[Signature]
 Operator's Signature

BROWARD COUNTY SO
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006475
 08/25/2016
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:35
Control Test	0.203	11:35
Air Blank	0.000	11:36
Control Test	0.203	11:37
Air Blank	0.000	11:37
Control Test	0.202	11:38
Air Blank	0.000	11:38

Control Test Stats
 Average 0.2027
 Std Dev 0.0006
 Rel Std Dev(%) 0.2849

[Signature]
 Operator's Signature

BROWARD COUNTY SO
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-006475
 08/25/2016
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:50
Control Test	0.079	11:51
Air Blank	0.000	11:51
Control Test	0.080	11:52
Air Blank	0.000	11:52
Control Test	0.080	11:52
Air Blank	0.000	11:53

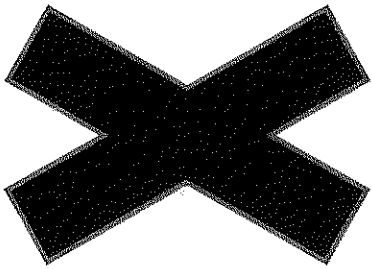
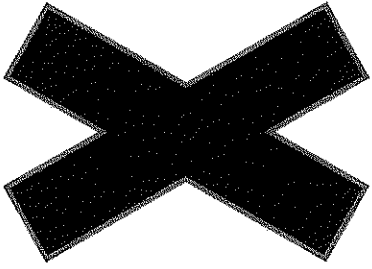
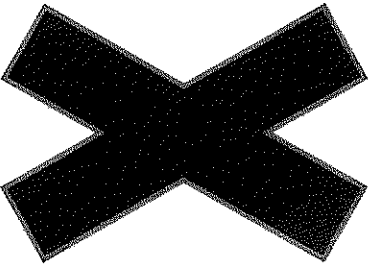
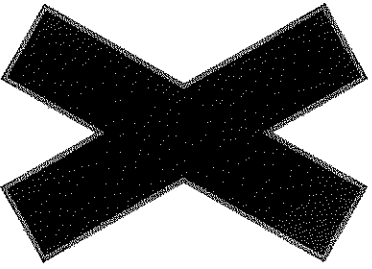
Control Test Stats
 Average 0.0797
 Std Dev 0.0006
 Rel Std Dev(%) 0.7247

[Signature]
 Operator's Signature

[Handwritten initials]

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Post Stabilities 2 nd Test	80-006475	Broward County Sheriff's Office	8/25/2016	

JK

0.05g/210L 0.047 to 0.053 <input type="checkbox"/>	0.08g/210L 0.077 to 0.083 <input type="checkbox"/>	0.20g/210L 0.194 to 0.206 <input checked="" type="checkbox"/>	DGS 0.08g/210L 0.077 to 0.083 <input type="checkbox"/>																																				
<p>Accidentally conducted two tests for the 0.20g/210L</p> <p>BROWARD COUNTY SO Intoxilyzer - Alcohol Analyzer Model 8000 SN 80-006475 J08/25/2016 Software: 0100.27</p> <table border="1"> <thead> <tr> <th>Test</th> <th>g/210L</th> <th>Time</th> </tr> </thead> <tbody> <tr> <td>Air Blank</td> <td>0.000</td> <td>11:46</td> </tr> <tr> <td>Control Test</td> <td>0.203</td> <td>11:47</td> </tr> <tr> <td>Air Blank</td> <td>0.000</td> <td>11:47</td> </tr> <tr> <td>Control Test</td> <td>0.203</td> <td>11:48</td> </tr> <tr> <td>Air Blank</td> <td>0.000</td> <td>11:48</td> </tr> <tr> <td>Control Test</td> <td>0.203</td> <td>11:49</td> </tr> <tr> <td>Air Blank</td> <td>0.000</td> <td>11:50</td> </tr> <tr> <td>Control Test Stats</td> <td></td> <td></td> </tr> <tr> <td>Average</td> <td>0.2030</td> <td></td> </tr> <tr> <td>Std Dev</td> <td>0.0000</td> <td></td> </tr> <tr> <td>Rel Std Dev(%)</td> <td>1.0000</td> <td></td> </tr> </tbody> </table> <p>Operator's Signature: <i>[Signature]</i></p>				Test	g/210L	Time	Air Blank	0.000	11:46	Control Test	0.203	11:47	Air Blank	0.000	11:47	Control Test	0.203	11:48	Air Blank	0.000	11:48	Control Test	0.203	11:49	Air Blank	0.000	11:50	Control Test Stats			Average	0.2030		Std Dev	0.0000		Rel Std Dev(%)	1.0000	
Test	g/210L	Time																																					
Air Blank	0.000	11:46																																					
Control Test	0.203	11:47																																					
Air Blank	0.000	11:47																																					
Control Test	0.203	11:48																																					
Air Blank	0.000	11:48																																					
Control Test	0.203	11:49																																					
Air Blank	0.000	11:50																																					
Control Test Stats																																							
Average	0.2030																																						
Std Dev	0.0000																																						
Rel Std Dev(%)	1.0000																																						
																																							

ggm