

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 12:50

Date of Inspection: 12/18/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:03417080A3<br>Exp: 03/05/2019 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.077   | 0.187 / 0.197   | 0.079   |
| 0.000                      | 0.049   | 0.079   | 0.198 / 0.197   | 0.079   |
| 0.000                      | 0.049   | 0.079   | 0.198 / 0.198   | 0.079   |

Number of Simulators Used: 5

**Remarks:**

20: Control Outside Tolerance LOOSE FITTING ON SIM. FIXED. CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name STEVE P. GASSEN

12/18/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 13:20

Date of Inspection: 11/27/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:03417080A3<br>Exp: 03/05/2019 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.078   | 0.205   | 0.080   |
| 0.000                      | 0.048   | 0.079   | 0.205   | 0.079   |
| 0.000                      | 0.048   | 0.078   | 0.203   | 0.079   |

Number of Simulators Used: 5

Remarks:  
CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

11/27/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 16:00

Date of Inspection: 10/31/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:03417080A3<br>Exp: 03/05/2019 |
|----------------------------|---|---|---|---|
| / 0.000                    | 0.049   | 0.079   | 0.203   | 0.079   |
| / 0.000                    | 0.049   | 0.080   | 0.204   | 0.079   |
| / 0.000                    | 0.050   | 0.079   | 0.205   | 0.080   |

Number of Simulators Used: 5

**Remarks:**

00: Ambient Fail. OPEN MOUTH ALCOHOL BOTTLE IN AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



STEVE P GASSEN

Signature and Printed Name

10/31/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 16:23

Date of Inspection: 09/29/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   | Yes |    |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |


| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#: 201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#: 201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 03417080A3<br>Exp: 03/05/2019 |
|----------------------------|--|--|--|--|
| 0.000                      | 0.048  | 0.079  | 0.204  | 0.078  |
| 0.000                      | 0.049  | 0.079  | 0.205  | 0.079  |
| 0.000                      | 0.048  | 0.079  | 0.204  | 0.079  |

Number of Simulators Used: 5

Remarks:  
Time-Date changed.

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

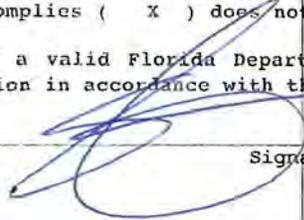

STEVE GASSEN

Signature and Printed Name

09/29/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT – INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 13:54

Date of Inspection: 08/28/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#: 201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#: 201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 03417080A3<br>Exp: 03/05/2019 |
|----------------------------|--|--|--|--|
| 0.000                      | 0.049  | 0.079  | 0.202  | 0.079  |
| 0.000                      | 0.050  | 0.079  | 0.203  | 0.080  |
| 0.000                      | 0.050  | 0.080  | 0.204  | 0.080  |

Number of Simulators Used: 5

**Remarks:**

CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



STEVE GASSEN

Signature and Printed Name

08/28/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 13:48

Date of Inspection: 07/24/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#: 201611B<br>Exp: 11/25/2018 | 0.20g/210L Test (g/210L)<br>Lot#: 201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 03417080A3<br>Exp: 03/05/2019 |
|----------------------------|--|--|--|--|
| 0.000                      | 0.049  | 0.079  | 0.200  | 0.079  |
| 0.000                      | 0.049  | 0.079  | 0.200  | 0.079  |
| 0.000                      | 0.049  | 0.079  | 0.201  | 0.079  |

Number of Simulators Used: 5

**Remarks:**

CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN  
Signature and Printed Name

07/24/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 09:42

Date of Inspection: 06/18/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:03417080A3<br>Exp: 03/05/2019 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.079   | 0.199   | 0.081   |
| 0.000                      | 0.049   | 0.079   | 0.199   | 0.080   |
| 0.000                      | 0.049   | 0.079   | 0.200   | 0.080   |

Number of Simulators Used: 5

Remarks:

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MICHAEL A ROQUE  
Signature and Printed Name

06/18/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 15:13

Date of Inspection: 06/01/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201603D<br>Exp: 03/08/2018 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201604C<br>Exp: 04/05/2018 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:03417080A3<br>Exp: 03/05/2019 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.049   | 0.079   | 0.200   | 0.080   |
| 0.000                      | 0.049   | 0.079   | 0.201   | 0.079   |
| 0.000                      | 0.049   | 0.079   | 0.201   | 0.080   |

Number of Simulators Used: 5

Remarks:  
CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE P GASSEN

Signature and Printed Name

06/01/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT – INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 16:05

Date of Inspection: 05/04/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#: 201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#: 201505A<br>Exp: 05/12/2017 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 03417080A3<br>Exp: 03/05/2019 |
|----------------------------|--|--|--|--|
| 0.000                      | 0.049  | 0.079  | 0.204  | 0.079  |
| 0.000                      | 0.050  | 0.079  | 0.204  | 0.080  |
| 0.000                      | 0.050  | 0.080  | 0.203  | 0.080  |


Number of Simulators Used: 5

**Remarks:**

CLEANED AREA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

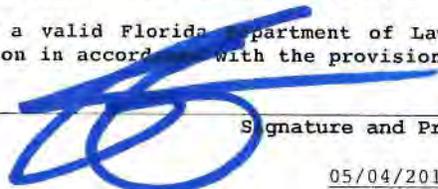  
\_\_\_\_\_  
Signature and Printed Name

STEVE GASSEN

05/04/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 09:46

Date of Inspection: 04/21/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201505A<br>Exp: 05/12/2017 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:11315080A2<br>Exp: 05/05/2017 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.000 / 0.079   | 0.203   | 0.077   |
| 0.000                      | 0.048   | 0.000 / 0.080   | 0.202   | 0.077   |
| 0.000                      | 0.048   | 0.000 / 0.079   | 0.203   | 0.077   |

Number of Simulators Used: 4

**Remarks:**

ACETONE STILL IN AREA AROUND INSTRUMENT. LEAK IN HOSE, HOSE RTUBE REPLACED

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



\_\_\_\_\_  
Signature and Printed Name STEVE GASSEN

04/21/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
APR 21 2017  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 09:46

Date of Inspection: 04/21/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201505A<br>Exp: 05/12/2017 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:11315080A2<br>Exp: 05/05/2017 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.000 / 0.079   | 0.203   | 0.077   |
| 0.000                      | 0.048   | 0.000 / 0.080   | 0.202   | 0.077   |
| 0.000                      | 0.048   | 0.000 / 0.079   | 0.203   | 0.077   |

Number of Simulators Used: 4

**Remarks:**

ACETONE STILL IN AREA AROUND INSTRUMENT. LEAK IN HOSE, HOSE RTUBE REPLACED

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name STEVE GASSEN

04/21/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 13:16

Date of Inspection: 02/27/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   | Yes |    |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#:201611B<br>Exp: 11/15/2018 | 0.20g/210L Test (g/210L)<br>Lot#:201505A<br>Exp: 05/12/2017 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:11315080A2<br>Exp: 05/05/2017 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.047   | 0.076   | 0.202   | 0.077   |
| 0.000                      | 0.049   | 0.078   | 0.202   | 0.077   |
| 0.000                      | 0.049   | 0.079   | 0.203   | 0.077   |

Number of Simulators Used: 4

**Remarks:**

Time-Date changed. Int Det: Ambient Fail ACETONE STILL PRESENT IN AREA.

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



STEVE GASSEN

Signature and Printed Name

02/27/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 16:41

Date of Inspection: 01/31/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#: 201502G<br>Exp: 02/24/2017 | 0.20g/210L Test (g/210L)<br>Lot#: 201505A<br>Exp: 05/12/2017 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 11315080A2<br>Exp: 05/05/2017 |
|----------------------------|--|--|--|--|
| 0.000                      | 0.047  | 0.077  | 0.196  | 0.079  |
| 0.000                      | 0.047  | 0.077  | 0.196  | 0.078  |
| 0.000                      | 0.048  | 0.078  | 0.197  | 0.078  |


Number of Simulators Used: 4

**Remarks:**

Int Det: Ambient Fail ACETONE STILL IN AIR.

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

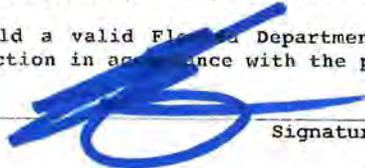

STEVE CASSEN

Signature and Printed Name

01/31/2017  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD  
Time of Inspection: 15:43

Date of Inspection: 01/31/2017

Serial Number: 80-001065  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      |     | No |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:201507A<br>Exp: 07/14/2017 | 0.08g/210L Test (g/210L)<br>Lot#:201502G<br>Exp: 02/24/2017 | 0.20g/210L Test (g/210L)<br>Lot#:<br>Exp: | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:<br>Exp: |
|----------------------------|---|---|---|--|
| 0.000                      | 0.047   | 0.113 / 0.072   |   |  |
| 0.000                      | 0.047   | 0.114 / 0.074   |   |  |
| 0.000                      | 0.047   | 0.113 / 0.075   |   |  |

Number of Simulators Used: 5

**Remarks:**

SIMULATOR HEATER WENT BAD, SWITCHED SIM, Control Outside To. SIMULATOR HEATER WENT BADCONTROL- OUTSID  
E TOLERANCE DUE TO EQUIPMENT PROBLEM.

The above instrument complies ( ) does not comply ( X ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Signature and Printed Name STEVE GASSEN

01/31/2017  
Date