

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 02:37

Date of Inspection: 12/01/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.049	0.078	0.198	0.082
0.000	0.048	0.078	0.199	0.082
0.000	0.049	0.078	0.199	0.082

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

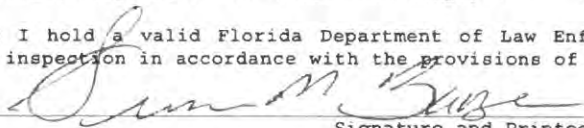

SUSAN M. BARGE

Signature and Printed Name

12/01/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:02

Date of Inspection: 11/05/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.050	0.079	0.198	0.081
0.000	0.049	0.079	0.197	0.082
0.000	0.050	0.078	0.197	0.081

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

11/05/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:03

Date of Inspection: 10/08/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.047	0.077	0.197	0.080
0.000	0.047	0.076	0.198	0.080
0.000	0.047	0.076	0.199	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

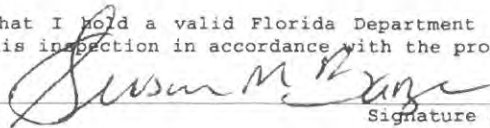

SUSAN M BARGE

Signature and Printed Name

10/08/2018

Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 10:54

Date of Inspection: 09/14/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.048	0.077	0.199	0.081
0.000	0.048	0.078	0.200	0.081
0.000	0.048	0.079	0.201	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

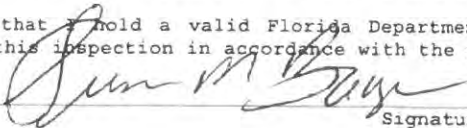

SUSAN M BARGE

Signature and Printed Name

09/14/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:32

Date of Inspection: 08/03/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 461951 Exp: 06/15/2019
0.000	0.048	0.078	0.199	0.081
0.000	0.048	0.078	0.199	0.081
0.000	0.048	0.078	0.199	0.081

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
 Signature and Printed Name

SUSAN M BARGE

08/03/2018  
 Date

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
JUL 18 2018  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 17:55

Date of Inspection: 07/06/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.050	0.079	0.199	0.082
0.000	0.049	0.079	0.201	0.082
0.000	0.049	0.079	0.200	0.082

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

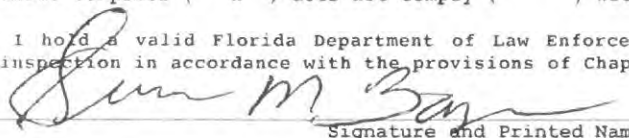  
 \_\_\_\_\_ SUSAN M BARGE  
 Signature and Printed Name

07/06/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 14:56

Date of Inspection: 05/01/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 461951 Exp: 06/15/2019
0.000	0.049	0.078	0.199	0.082
0.000	0.049	0.079	0.200	0.082
0.000	0.049	0.079	0.201	0.082

Number of Simulators Used: 5

Remarks:  
NONE NOTED

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

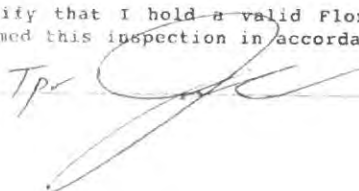

\_\_\_\_\_  
Signature and Printed Name JACOB A MOORE

05/01/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 21:28

Date of Inspection: 04/02/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.050	0.079	0.201	0.082
0.000	0.050	0.079	0.203	0.081
0.000	0.051	0.079	0.202	0.082

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



JOANNA N BOWMAN

Signature and Printed Name

04/02/2018  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 16:53

Date of Inspection: 02/17/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#: 201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#: 201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 461951 Exp: 06/15/2019
0.000	0.047	0.077	0.195	0.081
0.000	0.048	0.077	0.196	0.080
0.000	0.048	0.077	0.197	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

02/17/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HOLMES COUNTY SO  
Time of Inspection: 10:35

Date of Inspection: 02/02/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.048	0.079	0.198	0.081
0.000	0.048	0.079	0.199	0.081
0.000	0.048	0.079	0.199	0.081

Number of Simulators Used: 5

Remarks:  
Int Det: CHANGED SOLUTION.

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

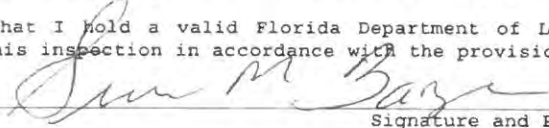

SUSAN M BARGE

Signature and Printed Name

02/02/2018  
Date

RECEIVED

# Florida Department of Law Enforcement Alcohol Testing Program

JAN 17 2018

FDLE  
Alcohol Testing Progra

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HOLMES COUNTY SO  
Time of Inspection: 13:17

Date of Inspection: 01/15/2018

Serial Number: 80-000784  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:461951 Exp: 06/15/2019
0.000	0.049	0.080	0.200	0.082
0.000	0.049	0.080	0.200	0.082
0.000	0.049	0.081	0.200	0.082

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

01/15/2018  
Date