

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 11:28

Date of Inspection: 09/14/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.076	0.198	0.081
0.000	0.048	0.078	0.201	0.081
0.000	0.047	0.078	0.201	0.081


Number of Simulators Used: 5

Remarks:

NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

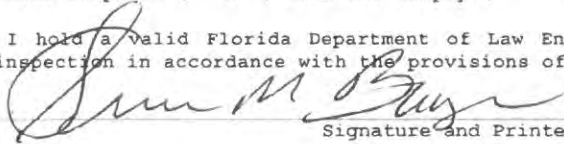

SUSAN N BARGE

Signature and Printed Name

09/14/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 10:45

Date of Inspection: 09/14/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.047			
0.000				
0.000				

Number of Simulators Used: 5


Remarks:

05: RFI Detect JAIL STAFF KEYED UP RADIO NEAR INTOX . 05Non-compliance:05.

♥ Screen clear before entering date
 Jail staff on other side of wall keyed up
 for radio causing an RFI on one intox. at the
 end of the table *SMB*

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE
 Signature and Printed Name

09/14/2018
 Date

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED
JUL 18 2018
Alcohol Testing Program
FDLE

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 15:53

Date of Inspection: 07/07/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.048	0.076	0.196	0.081
0.000	0.048	0.077	0.198	0.081
0.000	0.048	0.077	0.198	0.081

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

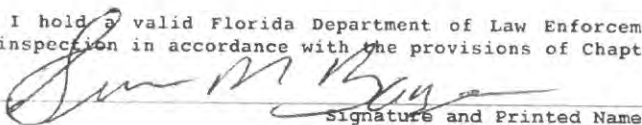

 signature and Printed Name

SUSAN M BARGE

07/07/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED
JUL 18 2018
FDLE
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP
Time of Inspection: 19:54

Date of Inspection: 05/08/2018

Serial Number: 80-000785
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) <i>201704A</i> Lot#: 201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.080
0.000	0.048	0.078	0.198	0.080
0.000	0.048	0.077	0.199	0.080

Number of Simulators Used: 5

Remarks:
NA

*0.08g/210L Test
Lot# 201704A
SMB*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M Barge

SUSAN M BARGE

Signature and Printed Name

05/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 13:46

Date of Inspection: 06/14/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.047	0.076	0.197	0.080
0.000	0.047	0.076	0.198	0.080
0.000	0.047	0.076	0.197	0.080


Number of Simulators Used: 5

Remarks:

NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

06/14/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 19:54

Date of Inspection: 05/08/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) <i>201709A</i> Lot#:201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.080
0.000	0.048	0.078	0.198	0.080
0.000	0.048	0.077	0.199	0.080

Number of Simulators Used: 5

Remarks:

NA

*0.08g/210L Test
Lot# 201709A
SMB*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M Barge

SUSAN M BARGE

Signature and Printed Name

05/08/2018

Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 19:54

Date of Inspection: 05/08/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.080
0.000	0.048	0.078	0.198	0.080
0.000	0.048	0.077	0.199	0.080

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

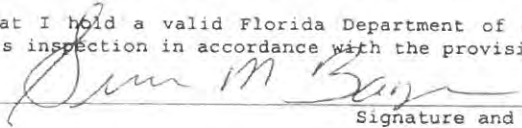

SUSAN M BARGE

Signature and Printed Name

05/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 19:20

Date of Inspection: 04/05/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.048	0.078	0.198	0.080
0.000	0.048	0.079	0.198	0.080
0.000	0.049	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:
NONE NOTED

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



JACOB A MOORE

Signature and Printed Name

04/05/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 02:00

Date of Inspection: 03/20/2018

Serial Number: 80-000785

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 07/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.049	0.078	0.199	0.081
0.000	0.049	0.078	0.200	0.080
0.000	0.049	0.079	0.200	0.080

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

03/20/2018

Date