

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DADE CITY PD
Time of Inspection: 16:38

Date of Inspection: 12/10/2020

Serial Number: 80-005477
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#: 201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 30219080A3 Exp: 01/05/2022
0.000	0.049	0.079	0.201	0.080
0.000	0.049	0.081	0.203	0.079
0.000	0.050	0.080	0.203	0.079

Number of Simulators Used: 4

Remarks:

Expired Mouth Alcohol Used

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 _____
Signature and Printed Name DEAN BALDWIN

12/10/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DADE CITY PD
Time of Inspection: 16:41

Date of Inspection: 11/17/2020

Serial Number: 80-005477
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:30219080A3 Exp: 01/05/2022
0.000	0.050	0.082	0.202	0.080
0.000	0.051	0.082	0.204	0.079
0.000	0.051	0.083	0.203	0.079


Number of Simulators Used: 4

Remarks:

Expired Mouth Alcohol Used

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 _____
Signature and Printed Name DEAN BALDWIN

11/17/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DADE CITY PD
Time of Inspection: 16:57

Date of Inspection: 10/14/2020

Serial Number: 80-005477
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:30219080A3 Exp: 01/05/2022
0.000	0.049	0.080	0.203	0.079
0.000	0.050	0.081	0.204	0.079
0.000	0.050	0.081	0.203	0.079

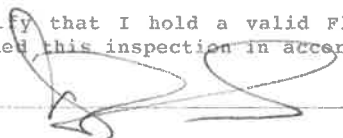
Number of Simulators Used: 4

Remarks:

Expired Mouth Alcohol Used

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DEAN BALDWIN

Signature and Printed Name

10/14/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT -- INTOXILYZER 8000

Agency: DADE CITY PD

Time of Inspection: 17:23

Date of Inspection: 09/23/2020

Serial Number: 80-005477

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:30219080A3 Exp: 01/05/2022
0.000	0.050	0.079	0.201	0.078
0.000	0.050	0.081	0.203	0.079
0.000	0.050	0.081	0.202	0.080

Number of Simulators Used: 4

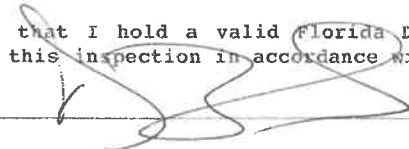
Remarks:

.20 EXPIRATION DATE OF 02/20/2021

EXPIRED MOUTH ALCOHOL USED

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name DEAN BALDWIN

09/23/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DADE CITY PD
Time of Inspection: 17:06

Date of Inspection: 08/25/2020

Serial Number: 80-005477
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:30219080A3 Exp: 01/05/2022
0.000	0.050	0.078	0.201	0.078
0.000	0.050	0.080	0.202	0.078
0.000	0.051	0.081	0.202	0.078

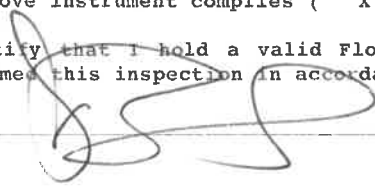
Number of Simulators Used: 4

Remarks:
BACK IN SERVICE

Expired Mouth Alcohol Used

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DEAN BALDWIN
Signature and Printed Name

08/25/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: DADE CITY PD
Time of Inspection: 09:45

Date of Inspection: 07/20/2020

Serial Number: 80-005477
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:24119080A1 Exp: 11/05/2021
0.000	0.050	0.080	0.203	0.079
0.000	0.050	0.081	0.203	0.079
0.000	0.050	0.081	0.203	0.079

Number of Simulators Used: 4

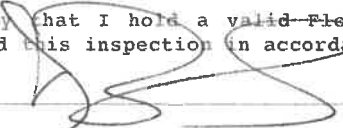
Remarks:

OUT FOR DEPARTMENT INSPECTION

Expanded Mouth Alcohol Used

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 _____ DEAN BALDWIN
Signature and Printed Name

07/20/2020
Date