



INSTRUMENT PROCESSING SHEET

Agency Ocala PD

S/N 80-006214

Florida Department of Law Enforcement

Date In 3/10/2020

DI Completion Date 4/1/2020

Ship P/U H/D CMI EE

Intake Performed By <u>DP</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input checked="" type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: _____ _____ _____		Quality Checks Performed By <u>DP</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>205</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP-102</u> 32 mm <u>0.144</u> (.139 - .169) 36 mm <u>0.164</u> (.156 - .190) 53 mm <u>0.234</u> (.228 - .278) 103 mm <u>0.500</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>28427</u> <input checked="" type="checkbox"/> Stability Checks		Flow Calibration Performed By _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																																																											
Final Release Date _____ _____		<table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td><u>SD1021</u></td> <td><u>201905A</u> <u>05-14-2021</u></td> </tr> <tr> <td>0.080</td> <td><u>DR1275</u></td> <td><u>201905B</u> <u>05-14-2021</u></td> </tr> <tr> <td>0.200</td> <td><u>SD1011</u></td> <td><u>201904D</u> <u>04-30-2021</u></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td><u>AG931603</u> <u>11-12-2021</u></td> </tr> </tbody> </table>		Simulator	Serial #	Lot #/Exp	0.050	<u>SD1021</u>	<u>201905A</u> <u>05-14-2021</u>	0.080	<u>DR1275</u>	<u>201905B</u> <u>05-14-2021</u>	0.200	<u>SD1011</u>	<u>201904D</u> <u>04-30-2021</u>	0.080 DGS	N/A	<u>AG931603</u> <u>11-12-2021</u>	Maintenance Performed By <u>SP</u> <input checked="" type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____																																												
Simulator	Serial #	Lot #/Exp																																																													
0.050	<u>SD1021</u>	<u>201905A</u> <u>05-14-2021</u>																																																													
0.080	<u>DR1275</u>	<u>201905B</u> <u>05-14-2021</u>																																																													
0.200	<u>SD1011</u>	<u>201904D</u> <u>04-30-2021</u>																																																													
0.080 DGS	N/A	<u>AG931603</u> <u>11-12-2021</u>																																																													
Calibration Adjustment Performed By _____ Barometric Pressure Gauge _____ ID # _____ <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.100</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.300</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table>		Simulator	Serial Number	Lot Number	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial Number	Lot Number	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Department Inspection Performed By <u>SP</u> Barometric Pressure ID# <u>30793</u> Gauge <u>1010</u> Instrument <u>1012</u> Mouth Alcohol Solution Lot # <u>2019-B</u> Acetone Stock Solution Lot # <u>2019-A</u> <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td><u>MP5086</u></td> </tr> <tr> <td>Interferent</td> <td><u>MP5087</u></td> </tr> <tr> <td>0.050</td> <td><u>MP5088</u></td> </tr> <tr> <td>0.080</td> <td><u>MP5089</u></td> </tr> <tr> <td>0.200</td> <td><u>MP5090</u></td> </tr> </tbody> </table>		Simulator	Serial Number	0.000	<u>MP5086</u>	Interferent	<u>MP5087</u>	0.050	<u>MP5088</u>	0.080	<u>MP5089</u>	0.200	<u>MP5090</u>
Simulator	Serial Number	Lot Number	Expiration																																																												
0.000		N/A	N/A																																																												
0.040																																																															
0.100																																																															
0.200																																																															
0.300																																																															
0.080 DGS	N/A																																																														
Simulator	Serial Number	Lot Number	Expiration																																																												
0.050																																																															
0.080																																																															
0.200																																																															
0.080 DGS	N/A																																																														
Simulator	Serial Number																																																														
0.000	<u>MP5086</u>																																																														
Interferent	<u>MP5087</u>																																																														
0.050	<u>MP5088</u>																																																														
0.080	<u>MP5089</u>																																																														
0.200	<u>MP5090</u>																																																														
Notes/Suggested Service: _____ _____ _____ _____ _____		Attachments <input checked="" type="checkbox"/> Form 41 <u>x2</u> <input checked="" type="checkbox"/> Stability Checks <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Post-Stability Checks <input type="checkbox"/> Flow Calibration <input checked="" type="checkbox"/> Form 40 <input type="checkbox"/> Other _____																																																													
		<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use																																																													
		Tech Review / Date _____ Admin Review / Date _____																																																													



Florida Department of Law Enforcement
Alcohol Testing Program
2729 Fort Knox Blvd.
Bldg. 2, Suite 1300
Tallahassee, FL 32308

Calibration Certificate

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006214, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006214</u>	UNCERTAINTY* \pm	
Owning Agency:	<u>Ocala Police Dept</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>04/01/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>12:42</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

04/01/2020 Date
 SHAYLA D PLATT,
Department Inspector

FDLE/ATP Form 69 January 2020
Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OCALA POLICE DEPT
Time of Inspection: 12:42

Date of Inspection: 04/01/2020

Serial Number: 80-006214
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG931603 Exp: 11/12/2021
0.000	0.047	0.078	0.199	0.078
0.000	0.047	0.078	0.198	0.077
0.000	0.048	0.079	0.199	0.077
0.000	0.048	0.078	0.199	0.077
0.000	0.048	0.079	0.199	0.077
0.000	0.047	0.078	0.200	0.077
0.000	0.047	0.079	0.200	0.077
0.000	0.048	0.079	0.200	0.078
0.000	0.047	0.079	0.200	0.078
0.000	0.048	0.078	0.199	0.077

Standard Deviations	0.0005	0.0005	0.0006	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0005 Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Shayla Platt

SHAYLA D PLATT

Signature and Printed Name

04/01/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OCALA POLICE DEPT
Time of Inspection: 21:50

Date of Inspection: 03/15/2020

Serial Number: 80-006214
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK		No	Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK		No
Alcohol Free Subject Test: 0.000		No	Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No	Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

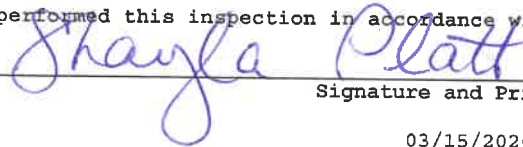
Standard Deviations				
---------------------	--	--	--	--

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: _____ Number of Simulators Used: _____

Remarks:
 ABORTING INSPECTION TO CHECK TIME *- Instrument requires battery change prior to inspection.*

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 SHAYLA D PLATT

 Signature and Printed Name

03/15/2020
Date

Stability Checks

OCALA POLICE DEPT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006214
03/13/2020
Software: 8100.27

OCALA POLICE DEPT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006214
03/13/2020
Software: 8100.27

OCALA POLICE DEPT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006214
03/13/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	14:14
Control Test	0.048	14:14
Air Blank	0.000	14:15
Control Test	0.047	14:16
Air Blank	0.000	14:16
Control Test	0.048	14:17
Air Blank	0.000	14:17
Control Test Stats		
Average	0.0477	
Std Dev	0.0006	
Rel Std Dev(%)	1.2112	

Test	g/210L	Time
Air Blank	0.000	14:20
Control Test	0.078	14:20
Air Blank	0.000	14:21
Control Test	0.078	14:21
Air Blank	0.000	14:22
Control Test	0.078	14:23
Air Blank	0.000	14:23
Control Test Stats		
Average	0.0780	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Test	g/210L	Time
Air Blank	0.000	14:25
Control Test	0.200	14:25
Air Blank	0.000	14:26
Control Test	0.199	14:27
Air Blank	0.000	14:27
Control Test	0.198	14:28
Air Blank	0.000	14:28
Control Test Stats		
Average	0.1990	
Std Dev	0.0010	
Rel Std Dev(%)	0.5025	

Wet

SS

Operator's Signature

SS

Operator's Signature

SS

Operator's Signature

OCALA POLICE DEPT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006214
03/13/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	14:30
Control Test	0.077	14:31
Air Blank	0.000	14:31
Control Test	0.077	14:31
Air Blank	0.000	14:32
Control Test	0.077	14:32
Air Blank	0.000	14:33
Control Test Stats		
Average	0.0770	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

OCALA POLICE DEPT
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-006214
04/01/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:07
Control Test	0.079	10:07
Air Blank	0.000	10:08
Control Test	0.079	10:08
Air Blank	0.000	10:09
Control Test	0.079	10:09
Air Blank	0.000	10:10
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Dry

DGS

SS

Operator's Signature

SP

Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OCALA POLICE DEPT
Time of Inspection: 12:03

Date of Inspection: 03/13/2020

Serial Number: 80-006214
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks:
BYPASSED AI TO OPERATE INSTRUMENT

N/A Instrument compliance not determined

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Israel Soto

ISRAEL SOTO

Signature and Printed Name

03/13/2020
Date