



INSTRUMENT PROCESSING SHEET

Agency Broward County SOS/N 80-006925

Florida Department of Law Enforcement

Date In 09/18/2020 DI Completion Date 09/21/2020 Ship P/U H/D CMI EE

Intake Performed By <u>MH</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: <u>Keyboard needs replaced</u>	Quality Checks Performed By <u>MH</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>199</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP 101</u> 32 mm <u>0.160</u> (.139 - .169) 36 mm <u>0.175</u> (.156 - .190) 53 mm <u>0.246</u> (.228 - .278) 103 mm <u>0.507</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>28199</u> <input checked="" type="checkbox"/> Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td>MP4863</td> <td>201905A 05/14/2021</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> <td>201905B 05/14/2021</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> <td>201904D 04/30/2021</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>AG003005 01/30/2022</td> </tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050	MP4863	201905A 05/14/2021	0.080	MP4864	201905B 05/14/2021	0.200	MP5097	201904D 04/30/2021	0.080 DGS	N/A	AG003005 01/30/2022	Flow Calibration Performed By _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)																																														
Simulator	Serial #	Lot #/Exp																																																													
0.050	MP4863	201905A 05/14/2021																																																													
0.080	MP4864	201905B 05/14/2021																																																													
0.200	MP5097	201904D 04/30/2021																																																													
0.080 DGS	N/A	AG003005 01/30/2022																																																													
Final Release Date FDLE Alcohol Testing Program Digitally signed by FDLE Alcohol Testing Program Date: 2020.09.22 15:31:26 -04'00'	Maintenance Performed By _____ <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____																																																														
Calibration Adjustment Performed By _____ ID # _____ Barometric Pressure Gauge <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.100</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.300</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table>		Simulator	Serial Number	Lot Number	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial Number	Lot Number	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Department Inspection Performed By <u>MH</u> Barometric Pressure ID# <u>68639</u> Gauge <u>1014</u> Instrument <u>1017</u> Mouth Alcohol Solution Lot # <u>2020-A</u> Acetone Stock Solution Lot # <u>2019-A</u> <table border="1" style="width:100%; border-collapse: collapse;"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td>SD1014</td> </tr> <tr> <td>Interferent</td> <td>SD1015</td> </tr> <tr> <td>0.050</td> <td>MP4863</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> </tr> <tr> <td>0.200</td> <td>MP5097</td> </tr> </tbody> </table>		Simulator	Serial Number	0.000	SD1014	Interferent	SD1015	0.050	MP4863	0.080	MP4864	0.200	MP5097
Simulator	Serial Number	Lot Number	Expiration																																																												
0.000		N/A	N/A																																																												
0.040																																																															
0.100																																																															
0.200																																																															
0.300																																																															
0.080 DGS	N/A																																																														
Simulator	Serial Number	Lot Number	Expiration																																																												
0.050																																																															
0.080																																																															
0.200																																																															
0.080 DGS	N/A																																																														
Simulator	Serial Number																																																														
0.000	SD1014																																																														
Interferent	SD1015																																																														
0.050	MP4863																																																														
0.080	MP4864																																																														
0.200	MP5097																																																														
Notes/Suggested Service: <u>Agency will replace keyboard.</u>		<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use																																																													
David Eliezer Reyes Rivera		Digitally signed by David Eliezer Reyes Rivera Date: 2020.09.22 09:59:21 -04'00'																																																													
Tech Review / Date		Admin Review / Date <u>2020.09.22 15:30:36 -04'00'</u>																																																													

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 12:07

Date of Inspection: 09/21/2020

Serial Number: 80-006925
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG003005 Exp: 01/30/2022
0.000	0.047	0.077	0.195	0.080
0.000	0.047	0.077	0.197	0.079
0.000	0.047	0.078	0.197	0.079
0.000	0.048	0.078	0.196	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.197	0.079
0.000	0.048	0.078	0.196	0.080
0.000	0.048	0.078	0.197	0.080


Standard Deviations	0.0004	0.0004	0.0006	0.0005
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:


The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

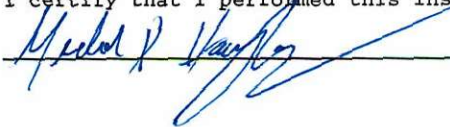 _____
Signature and Printed Name MICHAEL D HAUGHEY

09/21/2020
Date

DERR
Digitally signed by DERR Date: 2020.09.22 09:49:47 -0400

 2020.09.
22
15:29:59
-04'00'

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities	80-006925	Broward County SO	9/21/2020	MX

0.05g/210L	0.08g/210L	0.20g/210L	0.08g/210L
0.047 to 0.053 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>	0.194 to 0.206 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>

BROWARD COUNTY SO
Intoxilyzer - Alconol Analyzer
Model 8000 SN 80-016925
09/21/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:45
Control Test	0.047	09:46
Air Blank	0.000	09:46
Control Test	0.047	09:47
Air Blank	0.000	09:47
Control Test	0.047	09:48
Air Blank	0.000	09:49
Control Test Stats		
Average	0.0470	
Std Dev	0.0000	
Rel. Std Dev(%)	0.0000	

Operator's Signature

BROWARD COUNTY SO
Intoxilyzer - Alconol Analyzer
Model 8000 SN 80-016925
09/21/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:50
Control Test	0.077	09:51
Air Blank	0.000	09:51
Control Test	0.077	09:52
Air Blank	0.000	09:52
Control Test	0.077	09:53
Air Blank	0.000	09:54
Control Test Stats		
Average	0.0770	
Std Dev	0.0000	
Rel. Std Dev(%)	0.0000	

Operator's Signature

BROWARD COUNTY SO
Intoxilyzer - Alconol Analyzer
Model 8000 SN 80-016925
09/21/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:55
Control Test	0.195	09:55
Air Blank	0.000	09:56
Control Test	0.195	09:57
Air Blank	0.000	09:57
Control Test	0.196	09:58
Air Blank	0.000	09:58
Control Test Stats		
Average	0.1957	
Std Dev	0.0016	
Rel. Std Dev(%)	0.2951	

Operator's Signature


BROWARD COUNTY SO
Intoxilyzer - Alconol Analyzer
Model 8000 SN 80-016925
09/21/2020
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:59
Control Test	0.079	10:00
Air Blank	0.000	10:00
Control Test	0.078	10:00
Air Blank	0.000	10:01
Control Test	0.077	10:01
Air Blank	0.000	10:02
Control Test Stats		
Average	0.0780	
Std Dev	0.0010	
Rel. Std Dev(%)	1.2821	

Operator's Signature

DERR
Digitally signed
by DERR
Date: 2020.09.22
09:29:14-04'00'

2020.09.22 15:29:10
-04'00'



Florida Department of Law Enforcement
 Alcohol Testing Program
 4700 Terminal Drive, Suite 1
 Ft. Myers, FL 33907

Calibration Certificate

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006925, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006925</u>	UNCERTAINTY* ±	
Owning Agency:	<u>BROWARD COUNTY SO</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>09/21/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>12:07</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.

*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards. This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

09/21/2020

Date

MICHAEL D HAUGHEY,
 Department Inspector

FDLE/ATP Form 69 April 2020

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

DERR
Digitally signed by
 Date: 2020.09.22
 09:58:44 -0400

2020.09.22 15:28:39 -04'00'



INSTRUMENT PROCESSING SHEET

Agency Broward County Sheriff's Office

S/N 80-006925

Florida Department of Law Enforcement

Date In 03/09/2020 DI Completion Date 03/17/2020

Ship P/U H/D CMI EE

Intake Performed By <u>MX</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: _____ _____ _____	Quality Checks Performed By <u>MX</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value _____ <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP 101</u> 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>68639</u> <input checked="" type="checkbox"/> Stability Checks <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial #</th> <th>Lot #/Exp</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td>MP4863</td> <td>201905A 05/14/2021</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> <td>201905B 05/14/2021</td> </tr> <tr> <td>0.200</td> <td>SD3969</td> <td>201904D 04/30/2021</td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td>AG916501 06/14/2021</td> </tr> </tbody> </table>	Simulator	Serial #	Lot #/Exp	0.050	MP4863	201905A 05/14/2021	0.080	MP4864	201905B 05/14/2021	0.200	SD3969	201904D 04/30/2021	0.080 DGS	N/A	AG916501 06/14/2021	Flow Calibration Performed By <u>MX</u> Flow Column # <u>ATP 104</u> <input checked="" type="checkbox"/> 5L/min - 17mm <input checked="" type="checkbox"/> 15L/min - 53mm <input checked="" type="checkbox"/> 30L/min - 103mm <input checked="" type="checkbox"/> R-Value <u>227</u> <input checked="" type="checkbox"/> Post Calibration Verification (L/s) Flow Column # <u>ATP 101</u> 32 mm <u>0.152</u> (.139 - .169) 36 mm <u>0.167</u> (.156 - .190) 53 mm <u>0.242</u> (.228 - .278) 103 mm <u>0.507</u> (.447 - .547)
Simulator	Serial #	Lot #/Exp															
0.050	MP4863	201905A 05/14/2021															
0.080	MP4864	201905B 05/14/2021															
0.200	SD3969	201904D 04/30/2021															
0.080 DGS	N/A	AG916501 06/14/2021															
Final Release Date <p style="text-align: center;">FDLE</p> <p style="text-align: center;">APR 09 2020</p> <p style="text-align: center;">Alcohol Testing Program</p>	Maintenance Performed By _____ <input type="checkbox"/> Battery Replacement <input type="checkbox"/> Dry Gas Regulator Replacement <input type="checkbox"/> Breath Tube Replacement <input type="checkbox"/> Other _____	Temperature Checks Performed By <u>MX</u> <input checked="" type="checkbox"/> Lab Temp °C <u>22.52</u> External Digital Therm. ID#: <u>300504</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>MP4863</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>MP4864</u> <input checked="" type="checkbox"/> 34°C +/-2 Serial #: <u>SD1017</u>															

Calibration Adjustment Performed By _____ Barometric Pressure Gauge _____ ID # _____ <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td></td> <td>N/A</td> <td>N/A</td> </tr> <tr> <td>0.040</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.100</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.300</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table> <input type="checkbox"/> Post Calibration Adjustment Stability Checks <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> <th>Lot Number</th> <th>Expiration</th> </tr> </thead> <tbody> <tr> <td>0.050</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.200</td> <td></td> <td></td> <td></td> </tr> <tr> <td>0.080 DGS</td> <td>N/A</td> <td></td> <td></td> </tr> </tbody> </table>	Simulator	Serial Number	Lot Number	Expiration	0.000		N/A	N/A	0.040				0.100				0.200				0.300				0.080 DGS	N/A			Simulator	Serial Number	Lot Number	Expiration	0.050				0.080				0.200				0.080 DGS	N/A			Department Inspection Performed By <u>MX</u> Barometric Pressure ID# <u>28199</u> Gauge <u>1023</u> Instrument <u>1025</u> Mouth Alcohol Solution Lot # <u>2019-B</u> Acetone Stock Solution Lot # <u>2019-A</u> <table border="1"> <thead> <tr> <th>Simulator</th> <th>Serial Number</th> </tr> </thead> <tbody> <tr> <td>0.000</td> <td>SD1014</td> </tr> <tr> <td>Interferent</td> <td>SD1015</td> </tr> <tr> <td>0.050</td> <td>MP4863</td> </tr> <tr> <td>0.080</td> <td>MP4864</td> </tr> <tr> <td>0.200</td> <td>SD1017</td> </tr> </tbody> </table>	Simulator	Serial Number	0.000	SD1014	Interferent	SD1015	0.050	MP4863	0.080	MP4864	0.200	SD1017
Simulator	Serial Number	Lot Number	Expiration																																																										
0.000		N/A	N/A																																																										
0.040																																																													
0.100																																																													
0.200																																																													
0.300																																																													
0.080 DGS	N/A																																																												
Simulator	Serial Number	Lot Number	Expiration																																																										
0.050																																																													
0.080																																																													
0.200																																																													
0.080 DGS	N/A																																																												
Simulator	Serial Number																																																												
0.000	SD1014																																																												
Interferent	SD1015																																																												
0.050	MP4863																																																												
0.080	MP4864																																																												
0.200	SD1017																																																												
Attachments <input checked="" type="checkbox"/> Form 41 <input checked="" type="checkbox"/> Stability Checks <input checked="" type="checkbox"/> Calibration Certificate <input type="checkbox"/> Calibration Adjustment <input type="checkbox"/> Post-Stability Checks <input checked="" type="checkbox"/> Flow Calibration <input type="checkbox"/> Form 40 <input type="checkbox"/> Other _____	<input checked="" type="checkbox"/> Instrument Complies with Chapter 11D-8, FAC <input type="checkbox"/> Instrument Does Not Comply with Chapter 11D-8, FAC <input checked="" type="checkbox"/> Return to/Place into Evidentiary Use <input type="checkbox"/> Remain Out of Evidentiary Use <input checked="" type="checkbox"/> Conduct an Agency Inspection Before Evidentiary Use																																																												

Notes/Suggested Service: _____
 Repeated DI. Missed sim temp checks prior to first DI. Reran flow checks 3/17/2020, due to original flow data not saving.

 APPROVED 03/23/2020

SP 4/13/20 Brett Kirkland 4/7/2020
 Tech Review / Date Admin Review / Date

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 13:47

Date of Inspection: 03/17/2020

Serial Number: 80-006925
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG931603 Exp: 11/12/2021
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.078	0.196	0.078
0.000	0.047	0.077	0.196	0.078
0.000	0.047	0.077	0.195	0.078
0.000	0.047	0.077	0.196	0.078
0.000	0.047	0.077	0.197	0.079
0.000	0.047	0.077	0.196	0.079
0.000	0.047	0.077	0.196	0.078
0.000	0.048	0.077	0.196	0.078
0.000	0.048	0.077	0.197	0.078

Standard Deviations	0.0004	0.0003	0.0006	0.0004
---------------------	--------	--------	--------	--------


Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:

SP
TBK
4/7/2020

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MICHAEL D HAUGHEY

Signature and Printed Name

03/17/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 14:06

Date of Inspection: 03/11/2020

Serial Number: 80-006925
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201905A Exp: 05/14/2021	0.08g/210L Test (g/210L) Lot#:201905B Exp: 05/14/2021	0.20g/210L Test (g/210L) Lot#:201904D Exp: 04/30/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG931603 Exp: 11/12/2021
0.000	0.047	0.077	0.194	0.079
0.000	0.046	0.077	0.195	0.079
0.000	0.047	0.076	0.195	0.078
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.046	0.077	0.196	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.077	0.195	0.079
0.000	0.047	0.077	0.196	0.079

Standard Deviations	0.0004	0.0003	0.0005	0.0003
---------------------	--------	--------	--------	--------


Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

SP
TSK
4/7/2020

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



MICHAEL D HAUGHEY

Signature and Printed Name

03/11/2020
Date

TYPE OF TEST	SERIAL NUMBER	AGENCY	DATE	PERFORMED BY
Stabilities	80-006925	Broward County SO	3/11/2020	MK

0.05g/210L	0.08g/210L	0.20g/210L	DGS 0.08g/210L
0.047 to 0.053 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>	0.194 to 0.206 <input checked="" type="checkbox"/>	0.077 to 0.083 <input checked="" type="checkbox"/>

BROWARD COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000
03/11/2020
SN 80-006925
Software: 8100.27

Test g/210L Time

Air Blank 0.000 11:26
Control Test 0.047 11:27
Air Blank 0.000 11:27
Control Test 0.047 11:28
Air Blank 0.000 11:29
Control Test 0.047 11:29
Air Blank 0.000 11:30
Control Test Stats
Average 0.0470
Std Dev 0.0000
Rel Std Dev(%) 0.0000

BROWARD COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000
03/11/2020
SN 80-006925
Software: 8100.27

Test g/210L Time

Air Blank 0.000 11:31
Control Test 0.078 11:32
Air Blank 0.000 11:32
Control Test 0.077 11:33
Air Blank 0.000 11:34
Control Test 0.078 11:34
Air Blank 0.000 11:35
Control Test Stats
Average 0.0777
Std Dev 0.0005
Rel Std Dev(%) 0.7434

BROWARD COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000
03/11/2020
SN 80-006925
Software: 8100.27

Test g/210L Time

Air Blank 0.000 11:37
Control Test 0.195 11:37
Air Blank 0.000 11:38
Control Test 0.195 11:38
Air Blank 0.000 11:39
Control Test 0.195 11:39
Air Blank 0.000 11:40
Control Test Stats
Average 0.1950
Std Dev 0.0000
Rel Std Dev(%) 0.0000

DAS

BROWARD COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000
03/11/2020
SN 80-006925
Software: 8100.27

Test g/210L Time

Air Blank 0.000 11:42
Control Test 0.079 11:43
Air Blank 0.000 11:43
Control Test 0.077 11:43
Air Blank 0.000 11:44
Control Test 0.078 11:44
Air Blank 0.000 11:45
Control Test Stats
Average 0.0780
Std Dev 0.0010
Rel Std Dev(%) 1.2821

MK
Operator's Signature

MK
Operator's Signature

MK
Operator's Signature

MK
Operator's Signature

BSK
4/17/2020

Flow Calibration

03/11/2020

80-006925



MK

BROWARD COUNTY SO
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-016925
03/11/2020
Software: 8100.27

Flow Rate Calibration*****

1: Rate (Liters/min) = 5
 SQRT(Diff)) = 7.141
2: Rate (Liters/min) = 15
 SQRT(Diff)) = 11.832
3: Rate (Liters/min) = 30
 SQRT(Diff)) = 21.141
Dependent Data Scale Factor = 100000 L/min
Independent Data Scale Factor = 256
Rounded Slope = 688
Rounded Intercept = -688149
Correlation = 0.99732

SP
BK
4/7/2020



Calibration Certificate

Florida Department of Law Enforcement
Alcohol Testing Program
4700 Terminal Drive, Suite 1
Ft. Myers, FL 33907

This is to certify the calibration of Intoxilyzer 8000 serial number 80-006925, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-006925</u>	UNCERTAINTY* ±	
Owning Agency:	<u>BROWARD COUNTY SO</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>03/17/2020</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>13:47</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within ± 0.005 or 5%, whichever is greater, of the target alcohol concentration.
*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

03/17/2020

Date

MICHAEL DHAUGHEY,
Department Inspector

SP
BSK
4/7/2020

FDLE/ATP Form 69 January 2020

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality