

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ST PETERSBURG PD
Time of Inspection: 08:50

Date of Inspection: 12/24/2020

Serial Number: 80-001078
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:30219080A2 Exp: 12/05/2021
0.000	0.000 / 0.050	0.080	0.199	0.080
0.000	0.000 / 0.050	0.080	0.199	0.080
0.000	0.000 / 0.050	0.080	0.199	0.079

Number of Simulators Used: 5


Remarks:

05: Control Outside Tolerance.

2x Simulator top not Seated

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

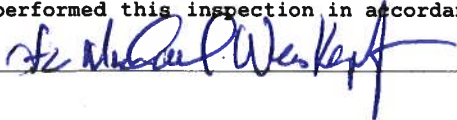

MICHAEL D WEISKOPF

Signature and Printed Name

12/24/2020
Date