

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD

Serial Number: 80-002989

Time of Inspection: 09:59

Date of Inspection: 06/15/2021

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.045	0.075	0.197	0.079
0.000	0.046	0.076	0.197	0.079
0.000	0.046	0.075	0.197	0.080

Number of Simulators Used: 5


Remarks:

SEE NOTES

*Remark created in error.
Instrument is in compliance
DK*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

06/15/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 13:17

Date of Inspection: 05/24/2021

Serial Number: 80-002989
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202005A Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34520080A1 Exp: 02/05/2023
0.000	0.046	0.077	0.198	0.080
0.000	0.046	0.077	0.199	0.080
0.000	0.046	0.077	0.199	0.080

Number of Simulators Used: 5


Remarks:

Int Det:LID NOT TIGHT.

Reconnected top of simulator and rechecked. No issues
DK

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DAVID KELLER

Signature and Printed Name

05/24/2021
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 09:40

Date of Inspection: 05/24/2021

Serial Number: 80-002989
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08g/210L Test (g/210L) Lot#:_____ Exp:_____	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____

Number of Simulators Used: 5


Remarks:

Time-Date changed. A F / M A:SEE NOTES. Non-compliance:SEE NOTES.

Instrument detected BAC. Contacted Department Inspector who advised to redo AFI No issues

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

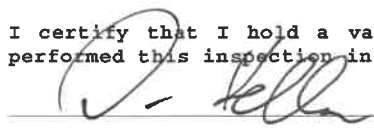

DAVID KELLER

Signature and Printed Name

05/24/2021
Date