

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 13:59

Date of Inspection: 03/14/2022

Serial Number: 80-000907
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1408275 Exp: 11/19/2023
0.000	0.048	0.079	0.199	0.080
0.000	0.048	0.080	0.199	0.080
0.000	0.048	0.080	0.199	0.080


Number of Simulators Used: 5

Remarks:

Contacted FDLE can test 3rd Time. Sent to FDLE for Follow-up

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

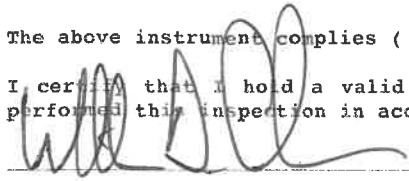

WILLIAM D COLEMAN

Signature and Printed Name

03/14/2022
Date