

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: INDIAN HARBOUR PD  
Time of Inspection: 10:17

Date of Inspection: 01/26/2022

Serial Number: 80-001263  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#: 202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#: 202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot #: 28021080A2 Exp: 12/05/2023
0.000	0.049	0.079	0.199	0.078
0.000	0.049	0.080	0.200	0.079
0.000	0.049	0.080	0.200	0.079


Number of Simulators Used: 5

Remarks:  
Int Det: Purge Fail.

*\* Purge Fail occurred due to oscillating fan being used and blowing near main unit. Was removed.*

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

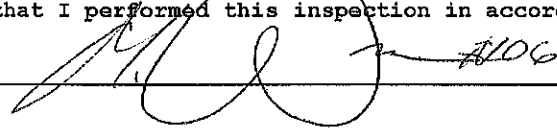

MATTHEW S WIMMER

Signature and Printed Name

01/26/2022

Date