

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency:
Time of Inspection:

Date of Inspection: 04-04-22

Serial Number: ~~80-1732~~
Software: 8100.27 001732

CHECK OR TEST	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		
Alcohol Free Subject Test: 0.000		
Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect		
Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Number of Simulators Used: _____

Remarks: Unable to bring instrument out of stand by due to DSP Errors. Reported issue to Department Inspector and sent to FOLE and then to CMT. Inspection could not be completed.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

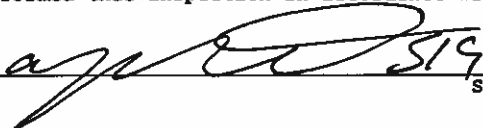

Signature and Printed Name

Date