

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 11:48

Date of Inspection: 03/23/2022

Serial Number: 80-006565
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202007A Exp: 07/21/2022	0.20g/210L Test (g/210L) Lot#:202106B Exp: 05/12/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1303107 Exp: 03/28/2023
0.000	0.049	0.080	0.200	0.080
0.000	0.049	0.080	0.200	0.080
0.000	0.049	0.080	0.201	0.080

Number of Simulators Used: 5


Remarks:

Int Det: RFI Detect. LOCATED RFI REMOVED IT

20 Reference Solution Entered incorrectly: Should read 202005A

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

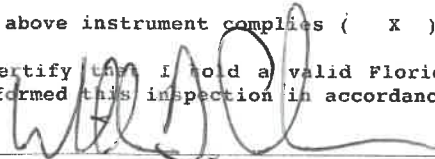

WILLIAM D COLEMAN

Signature and Printed Name

03/23/2022
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO
Time of Inspection: 10:46

Date of Inspection: 03/23/2022

Serial Number: 80-006565
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.050 / 0.050			
0.000	0.051 / 0.051			
0.000	0.051 / RFI			

Number of Simulators Used: 5


Remarks:

05: RFI Detect, RFI Detect. Non-compliance: RFI DETECT.

Located RFI Source and Removed

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

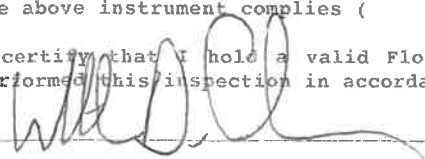

WILLIAM D. COLEMAN

Signature and Printed Name

03/23/2022
Date