

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: KENNEDY SPACE CENTER
Time of Inspection: 09:30

Date of Inspection: 05/18/2022

Serial Number: 80-006621
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202101C Exp: 01/12/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:19021080A2 Exp: 09/05/2023
0.000	0.045	0.076	0.195	0.080
0.000	0.045	0.077	0.196	0.080
0.000	0.045	0.077	0.196	0.080

Number of Simulators Used: 5

Remarks: *I provided AN ALCOHOL FREE BREATH SAMPLE when prompted. The instrument went through its cycle, then prompted me to provide a sample of mouth alcohol. After reviewing that phase of the inspection I saw that the ALCOHOL FREE RECORDED 0.000 AND the mouth ALCOHOL showed slope Not met. After printing the AFFIDAVIT I noticed the ALCOHOL FREE test indicated NO in the NO box, which I realized WAS NOT correct. A second inspection was performed with no problems.*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

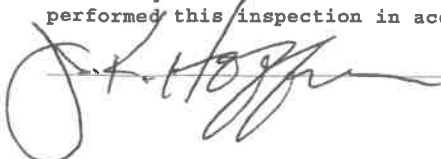

JOHN K HOFFMANN
Signature and Printed Name

05/18/2022
Date