



Agency Osceola Corrections

S/N 80-000968

Date In 01/20/22

DI Completion Date 01/21/22

☒ Ship   ☐ P/U   ☐ H/D   ☐ CMI   ☐ EE

## Calibration Adjustment

By

☐ Post Calibration Adjustment Stability Checks

Notes/Suggested Service:

## Department Inspection

By RAW

## Attachments

- ☒ Instrument Complies with Chapter 11D-8, FAC
- ☐ Instrument Does Not Comply with Chapter 11D-8, FAC
- ☒ Return to/Place into Evidentiary Use
- ☐ Remain Out of Evidentiary Use
- ☒ Conduct an Agency Inspection Before Evidentiary Use

Israel Soto

Digitally signed by Israel Soto  
Date: 2022.01.21 12:49:39  
+05'00'

Tech Review / Date

Admin Review/ Date 05'00'

# Florida Department of Law Enforcement Alcohol Testing Program

## DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS  
Time of Inspection: 12:10

Date of Inspection: 01/21/2022

Serial Number: 80-000968  
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202010A Exp: 10/05/2022	0.08g/210L Test (g/210L) Lot#:202010B Exp: 10/05/2022	0.20g/210L Test (g/210L) Lot#:202010D Exp: 10/06/2022	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG113403 Exp: 05/14/2023
0.000	0.049	0.079	0.200	0.081
0.000	0.049	0.079	0.199	0.081
0.000	0.049	0.079	0.199	0.081
0.000	0.049	0.079	0.199	0.081
0.000	0.049	0.080	0.200	0.080
0.000	0.049	0.079	0.200	0.080
0.000	0.049	0.080	0.199	0.081
0.000	0.050	0.079	0.200	0.080
0.000	0.050	0.079	0.200	0.081
0.000	0.050	0.079	0.200	0.081

Standard Deviations	0.0004	0.0004	0.0005	0.0004
---------------------	--------	--------	--------	--------

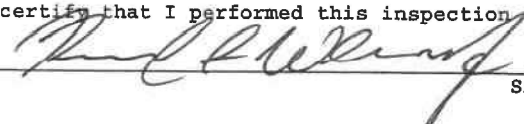
Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

**Remarks:**

A F / M A: Range Exceeded. TOO MUCH MA. -RAW,01/21/22.

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
 Signature and Printed Name

RICHARD A WILLIAMS

01/21/2022  
Date

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
01/21/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:38
Control Test	0.049	09:38
Air Blank	0.000	09:39
Control Test	0.049	09:40
Air Blank	0.000	09:40
Control Test	0.049	09:41
Air Blank	0.000	09:41
Control Test Stats		
Average	0.0490	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

.05

RAW

Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
01/21/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:43
Control Test	0.079	09:44
Air Blank	0.000	09:44
Control Test	0.080	09:45
Air Blank	0.000	09:45
Control Test	0.080	09:46
Air Blank	0.000	09:47
Control Test Stats		
Average	0.0797	
Std Dev	0.0006	
Rel Std Dev(%)	0.7247	

.08  
wet

RAW

Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
01/21/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:50
Control Test	0.200	09:51
Air Blank	0.000	09:51
Control Test	0.199	09:52
Air Blank	0.000	09:53
Control Test	0.199	09:53
Air Blank	0.000	09:54
Control Test Stats		
Average	0.1993	
Std Dev	0.0006	
Rel Std Dev(%)	0.2896	

.20

RAW

Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
01/21/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	09:55
Control Test	0.080	09:56
Air Blank	0.000	09:56
Control Test	0.081	09:56
Air Blank	0.000	09:57
Control Test	0.081	09:57
Air Blank	0.000	09:58
Control Test Stats		
Average	0.0807	
Std Dev	0.0006	
Rel Std Dev(%)	0.7157	

.08  
DAS

RAW

Operator's Signature

Stability Checks

80-000968

01/21/22

RAW



# Calibration Certificate

Florida Department of Law Enforcement  
Alcohol Testing Program  
2729 Fort Knox Blvd.  
Bldg. 2, Suite 1300  
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000968, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000968</u>	UNCERTAINTY* $\pm$
Owning Agency:	<u>OSCEOLA CORRECTIONS</u>	0.050 g/ 210 L 0.004
Calibration Date:	<u>01/21/2022</u>	0.080 g/ 210 L 0.004
Calibration Time:	<u>12:10</u>	0.200 g/ 210 L 0.007
		0.080 g/ 210 L Dry Gas Control 0.005

All results are reported in g/210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within  $\pm 0.005$  or 5%, whichever is greater, of the target alcohol concentration.

\*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ( $k=3$ ).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

## TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

Richard A  
Williams  
Digitally signed by Richard A  
Williams  
Date: 2022.01.21 12:33:33  
-05'00'

01/21/2022

Date

RICHARD A WILLIAMS,  
Department Inspector

FDLE/ATP Form 69 January 2022

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality



## Agency Osceola Corrections

S/N 80-000968

Date In 12/12/2022      DI Completion Date 12/15/2022

☒ Ship ☐ P/U ☐ H/D ☐ CMI ☐ EE

## Calibration Adjustment

By

Barometric Pressure Gauge \_\_\_\_\_ ID # \_\_\_\_\_

### ☐ Post Calibration Adjustment Stability Checks

Notes/Suggested Service:

## Department Inspection

By PN

Barometric Pressure ID# 28421

Gauge 1009	Instrument 1009
------------	-----------------

Mouth Alcohol Solution Lot # 2022-A

Acetone Stock Solution Lot # 2022-B

## Attachments

- |   |  |
|---|--|
| <input checked="" type="checkbox"/> Form 41                 | <input type="checkbox"/> Post-Stability Checks |
| <input checked="" type="checkbox"/> Stability Checks        | <input type="checkbox"/> Flow Calibration      |
| <input checked="" type="checkbox"/> Calibration Certificate | <input type="checkbox"/> Form 40               |
| <input type="checkbox"/> Calibration Adjustment             | <input type="checkbox"/> Other                 |

- ☒ Instrument Complies with Chapter 11D-8, FAC
  - ☐ Instrument Does Not Comply with Chapter 11D-8, FAC
  - ☒ Return to/Place into Evidentiary Use
  - ☐ Remain Out of Evidentiary Use
  - ☒ Conduct an Agency Inspection Before Evidentiary Use

Taylor  
Gutschow

Digitally signed by Taylor  
Gutschow  
Date: 2022.12.16 08:49:35  
,05'00'

Israel Soto

Digitally signed by Israel Soto  
Date: 2022.12.16 10:26:38 -05'00'

Tech Review / Date

Admin Review / Date

## STABILITY CHECKS


80-000968

12/14/2022

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
12/14/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:09
Control Test	0.049	15:10
Air Blank	0.000	15:10
Control Test	0.048	15:11
Air Blank	0.000	15:11
Control Test	0.048	15:12
Air Blank	0.000	15:13
Control Test Stats		
Average	0.0483	
Std Dev	0.0006	
Rel Std Dev(%)	1.1945	


0.05 g/210L

  
Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
12/14/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:14
Control Test	0.078	15:15
Air Blank	0.000	15:15
Control Test	0.077	15:16
Air Blank	0.000	15:16
Control Test	0.078	15:17
Air Blank	0.000	15:17
Control Test Stats		
Average	0.0777	
Std Dev	0.0006	
Rel Std Dev(%)	0.7434	


0.08 g/210L

  
Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
12/14/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:19
Control Test	0.198	15:19
Air Blank	0.000	15:20
Control Test	0.198	15:21
Air Blank	0.000	15:21
Control Test	0.199	15:22
Air Blank	0.000	15:22
Control Test Stats		
Average	0.1983	
Std Dev	0.0006	
Rel Std Dev(%)	0.2911	

0.20 g/210L

  
Operator's Signature

OSCEOLA CORRECTIONS  
Intoxilyzer - Alcohol Analyzer  
Model 8000 SN 80-000968  
12/14/2022  
Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	15:24
Control Test	0.078	15:24
Air Blank	0.000	15:25
Control Test	0.077	15:25
Air Blank	0.000	15:25
Control Test	0.078	15:26
Air Blank	0.000	15:26
Control Test Stats		
Average	0.0777	
Std Dev	0.0006	
Rel Std Dev(%)	0.7434	

DGS 0.08 g/210L

  
Operator's Signature



# Florida Department of Law Enforcement Alcohol Testing Program

## DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS  
Time of Inspection: 11:23

Date of Inspection: 12/15/2022

Serial Number: 80-000968  
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202201C Exp: 01/11/2024	0.08g/210L Test (g/210L) Lot#:202201D Exp: 01/18/2024	0.20g/210L Test (g/210L) Lot#:202201E Exp: 01/18/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG229803 Exp: 10/25/2024
0.000	0.048	0.077	0.197	0.077
0.000	0.048	0.077	0.198	0.078
0.000	0.048	0.077	0.198	0.077
0.000	0.048	0.077	0.197	0.078
0.000	0.048	0.077	0.197	0.078
0.000	0.048	0.077	0.198	0.078
0.000	0.048	0.078	0.198	0.078
0.000	0.048	0.077	0.198	0.078
0.000	0.048	0.078	0.198	0.078
0.000	0.048	0.078	0.198	0.078

Standard Deviations	0.0000	0.0004	0.0004	0.0004
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



PHIL NICODEMO

Signature and Printed Name

12/15/2022  
Date



## Calibration Certificate

Florida Department of Law Enforcement  
Alcohol Testing Program  
2331 Phillips Road.  
Suite B1032  
Tallahassee, FL 32308

This is to certify the calibration of Intoxilyzer 8000 serial number 80-000968, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-000968</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>OSCEOLA CORRECTIONS</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>12/15/2022</u>	0.080 g/ 210 L	0.004
Calibration Time:	<u>11:23</u>	0.200 g/ 210 L	0.007
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.

Bias is limited by calibration acceptance criteria. All calibration results must be within  $\pm 0.005$  or 5%, whichever is greater, of the target alcohol concentration.

\*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence ( $k=3$ ).

The instrument results before and after any adjustment are found in the associated pre and post stability checks.

### TRACEABILITY INFORMATION

This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Simulator temperatures are checked with NIST traceable digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the use of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

12/15/2022

Date

Phil Nicodemo

PHIL NICODEMO,  
Department Inspector

Digitally signed by Phil  
Nicodemo  
Date: 2022.12.15 14:54:14  
-05'00'

FDLE/ATP Form 69 March 2022

Issuing Authority: Alcohol Testing Program

Service • Integrity • Respect • Quality

Page 1 of 1