



Florida Department of  
Law Enforcement

## AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Manatee CSO

Instrument Serial Number: 80-006634

### AGENCY INSPECTION DISCREPENCY

Agency Inspector: William Coleman

Inspection Date: 02/06/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☐ 0.050 g/210L ☒ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Other Electronic Data Review/Comments:

### REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.05.17 09:17:37 -04'00'

05/17/2023

Signature of Alcohol Testing Program Staff Member

Date

Ammended

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO  
Time of Inspection: 14:33

Date of Inspection: 02/06/2023

Serial Number: 80-006634  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558895 Exp: 10/03/2025
0.000	0.048	0.078	0.199	0.082
0.000	0.048	0.078	0.198	0.082
0.000	0.048	0.078	0.199	0.082


Number of Simulators Used: 5

Remarks:

Incorrect Lot # and Expiration entered. Corrected above. (WOC)

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

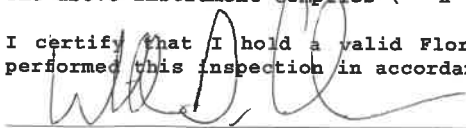

WILLIAM COLEMAN

Signature and Printed Name

02/06/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO  
Time of Inspection: 14:12

Date of Inspection: 05/15/2023

Serial Number: 80-006634  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558875 Exp: 10/03/2025
0.000 / 0.000	0.049	0.079	0.199	0.082
/ 0.000	0.049	0.078	0.199	0.081
/ 0.000	0.049	0.079	0.200	0.082

Number of Simulators Used: 5


**Remarks:**

00: RFI Detect.

Located source of RFI, removed and repeated test.

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

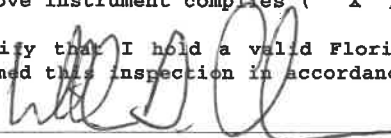

WILLIAM D COLEMAN

Signature and Printed Name

05/15/2023  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: MANATEE COUNTY SO  
Time of Inspection: 14:19

Date of Inspection: 04/10/2023

Serial Number: 80-006634  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#:202108D Exp: 08/17/2023	0.20g/210L Test (g/210L) Lot#:202106B Exp: 06/22/2023	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402558895 Exp: 10/03/2025
0.000	0.048 / 0.048	0.078	0.199	0.082
0.000	0.048 / 0.048	0.078	0.199	0.082
0.000	RFI / 0.049	0.078	0.199	0.082


Number of Simulators Used: 5

Remarks:

Time-Date changed. 05: RFI Detect. RFI source located and removed. Re-started the test with no further issues.

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

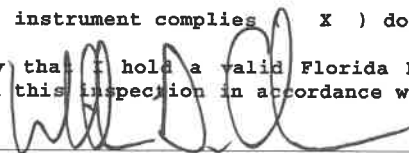

WILLIAM D COLEMAN

Signature and Printed Name

04/10/2023  
Date