

# Amendment

## Florida Department of Law Enforcement Alcohol Testing Program

### AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY S.O.  
Time of Inspection: 11:45

Date of Inspection: 10/04/2023

Serial Number: 80-007107  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#: 202206B-<br>Exp: 06/14/2024 | 0.08g/210L Test (g/210L)<br>Lot#: 202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#: 202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 402477283<br>Exp: 06/24/2025 |
|----------------------------|---|--|--|---|
| 0.000                      | 0.048   | 0.078  | 0.198  | 0.082   |
| 0.000                      | 0.048   | 0.079  | 0.199  | 0.081   |
| 0.000                      | 0.049   | 0.078  | 0.199  | 0.081   |

Number of Simulators Used: 5

**Remarks:**

J. GUZMAN IN TRAINING.

04  
11/5/2023

0.05 g/210 L Test  
LOT #: 202303J  
Exp: 03/28/2025

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*[Handwritten Signature]*

ANAYA S FRAZIER

Signature and Printed Name

10/04/2023  
Date



Florida Department of  
Law Enforcement

## AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Broward CSO

Instrument Serial Number: 80-007107

### AGENCY INSPECTION DISCREPENCY

Agency Inspector: Anaya Frazier

Inspection Date: 09/06/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☒ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Other Electronic Data Review/Comments: The 0.05 ARS lot number is mistyped.

### REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.10.31 14:34:48 -04'00'

10/31/2023

Signature of Alcohol Testing Program Staff Member

Date

**AMENDMENT**  
Florida Department of Law Enforcement  
Alcohol Testing Program

**AGENCY INSPECTION REPORT - INTOXILYZER 8000**

Agency: BROWARD COUNTY S.O.

Time of Inspection: 11:25

Date of Inspection: 09/06/2023

Serial Number: 80-007107

Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br><del>Lot#: 2022033</del><br>Exp: 03/28/2025 | 0.08g/210L Test (g/210L)<br>Lot#: 202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#: 202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#: 402477283<br>Exp: 09/06/2023 |
|----------------------------|---|--|--|---|
| 0.000                      | 0.048   | 0.078  | 0.196  | 0.081   |
| 0.000                      | 0.049   | 0.078  | 0.195  | 0.081   |
| 0.000                      | 0.049   | 0.078  | 0.195  | 0.081   |

Number of Simulators Used: 5

Remarks:

J. GUZMAN IN TRAINING.

The above instrument complies ( ☒ ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

ANAYA S FRAZIER

09/06/2023  
Date

# AMENDMENT

## Florida Department of Law Enforcement Alcohol Testing Program

### AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY S.O.  
Time of Inspection: 10:54

Date of Inspection: 07/05/2023

Serial Number: 80-007107  
Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402477283<br>Exp: 06/07/2023 Q4 |
|----------------------------|---|---|---|---|
| 0.000                      | 0.048   | 0.078   | 0.199   | 0.081   |
| 0.000                      | 0.049   | 0.078   | 0.199   | 0.081   |
| 0.000                      | 0.049   | 0.079   | 0.199   | 0.081   |

Number of Simulators Used: 5

**Remarks:**

J. GUZMAN IN TRAINING.

*Incorrect Exp. Date for 0.08g/210L Dry Gas Standard. Correct Exp. Date is 06/24/2025. Q4*

The above instrument complies ( ☒ ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

ANAYA S FRAZIER

Signature and Printed Name

07/05/2023  
Date



Florida Department of  
Law Enforcement

## AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Broward CSO

Instrument Serial Number: 80-007107

### AGENCY INSPECTION DISCREPANCY

Agency Inspector: Anaya Frazier

Inspection Date: 02/01/2023

☒ A test was repeated without reason for repeat or the corrective action given

☒ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Lot Number and/or Expiration Date for Standards entered incorrectly

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Other Electronic Data Review/Comments:

### REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.05.17 11:11:23 -04'00'

05/17/2023

Signature of Alcohol Testing Program Staff Member

Date



# Amendment

## Florida Department of Law Enforcement Alcohol Testing Program

### AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY S.O.

Time of Inspection: 14:50

Date of Inspection: 02/01/2023

Serial Number: 80-007107

Software: 8100.27

| Check or Test                               | YES | NO |
|---|-----|----|
| Date and/or Time Adjusted                   |     | No |
| Diagnostic Check (Pre-Inspection): OK       | Yes |    |
| Alcohol Free Subject Test: 0.000            | Yes |    |
| Mouth Alcohol Test: Slope Not Met           | Yes |    |
| Interferent Detect Test: Interferent Detect | Yes |    |
| Diagnostic Check (Post-Inspection): OK      | Yes |    |

| Alcohol Free Test (g/210L) | 0.05g/210L Test (g/210L)<br>Lot#:202112A<br>Exp: 12/07/2023 | 0.08g/210L Test (g/210L)<br>Lot#:202206B<br>Exp: 06/14/2024 | 0.20g/210L Test (g/210L)<br>Lot#:202206C<br>Exp: 06/15/2024 | 0.08 g/210L Dry Gas Std Test (g/210L)<br>Lot#:402477283<br>Exp: 06/24/2025 |
|----------------------------|---|---|---|--|
| 0.000                      | 0.048   | 0.077   | 0.198   | 0.081  |
| 0.000                      | 0.048   | 0.077   | 0.198   | 0.081  |
| 0.000                      | 0.048   | 0.077   | 0.198   | 0.081  |

Number of Simulators Used: 5


Remarks:

A F / M A: .J GUZMAN IN TRAINING

TOO MUCH MOUTH ALCOHOL QA  
5/20/2023

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

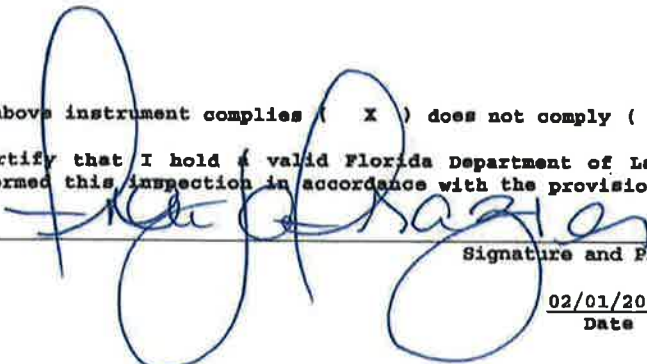

ANAYA S FRAZIER

Signature and Printed Name

02/01/2023  
Date