

AMENDMENT

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 12:27

Date of Inspection: 10/04/2023

Serial Number: 80-007434
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202203J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402623828 Exp: 12/22/2025
0.000	0.050	0.080	0.202	0.079
0.000	0.050	0.080	0.202	0.079
0.000	0.050	0.080	0.202	0.080

Number of Simulators Used: 5

Remarks:
J GUZMAN IN TRAINING

OA
11/5/2023 0.05 g/210L Test
LOT # 202303J

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 ANAYA S FRAZIER
Signature and Printed Name

10/04/2023
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Broward CSO

Instrument Serial Number: 80-007434

AGENCY INSPECTION DISCREPANCY

Agency Inspector: Anaya Frazier

Inspection Date: 09/06/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☒ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Other Electronic Data Review/Comments: The 0.05 ARS lot number is mistyped.

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.10.31 14:36:09 -04'00'

Signature of Alcohol Testing Program Staff Member

10/31/2023

Date

AMENDMENT

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT – INTOXILYZER 8000

Agency: BROWARD COUNTY SO

Time of Inspection: 11:28

Date of Inspection: 09/06/2023

Serial Number: 80-007434

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202203J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Drv Gas Std Test (g/210L) Lot#: 402623828 Exp: 12/22/2025
0.000	0.050	0.080	0.200	0.079
0.000	0.050	0.080	0.200	0.079
0.000	0.050	0.080	0.200	0.079

Number of Simulators Used: 5

Remarks:

A F / M A: RFI Detect.UNKNOWN SOURCE.JGUZMAN IN TRAINING

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 ANAYA S FRAZIER
Signature and Printed Name

09/06/2023
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Broward CSO

Instrument Serial Number: 80-007434

AGENCY INSPECTION DISCREPANCY

Agency Inspector: Anaya Frazier

Inspection Date: 07/05/2023

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☒ 0.050 g/210L ☒ 0.080 g/210L ☒ 0.200 g/210L ☒ 0.080 g/210L Dry Gas

☒ Other Electronic Data Review/Comments: The lot numbers of the 0.05, 0.08, and 0.20 ARS are mistyped. The expiration date of the DGS is mistyped.

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.10.30 13:05:04 -04'00'

10/30/2023

Signature of Alcohol Testing Program Staff Member

Date

AMENDMENT

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 11:40

Date of Inspection: 07/05/2023

Serial Number: 80-007434
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202-112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202-206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202-206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402623828 Exp: 07/05/2023
0.000	0.049	0.080	0.203	0.080
0.000	0.049	0.080	0.203	0.080
0.000	0.049	0.080	0.203	0.080

Number of Simulators Used: 5

Remarks:
A

0.05g
LOT #: 202112A


0.08g
LOT #: 202206B

0.20g
LOT #
202206C

0.08g Dry Gas Standard:
Expiration: 06/24/2025

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

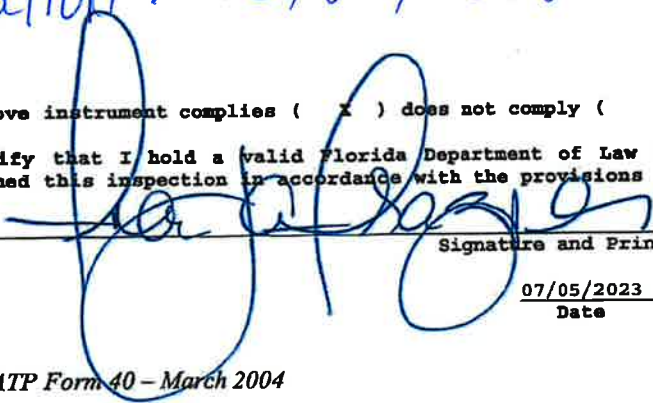

ANAYA S FRAZIER

Signature and Printed Name

07/05/2023
Date



Florida Department of
Law Enforcement

**AGENCY INSPECTION AND OTHER
ELECTRONIC DATA REVIEW**

Agency: Broward CSO

Instrument Serial Number: 80-007434

AGENCY INSPECTION DISCREPENCY

Agency Inspector: Anaya Frazier

Inspection Date: 02/01/2023

☒ **A test was repeated without reason for repeat or the corrective action given**

☐ Alcohol Free/Mouth Alcohol ☒ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Agency Inspection not conducted for calendar month**

☐ **Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection**

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Lot Number and/or Expiration Date for Standards entered incorrectly**

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ **Other Electronic Data Review/Comments:**

REQUESTED CORRECTIVE ACTION

☒ **Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector**

☐ **Provide written explanation regarding referenced item(s) to Department Inspector**

☐ **Remove instrument from evidentiary use until otherwise directed by the Department**

☐ **Other:**

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2023.05.17 11:16:11 -04'00'

05/17/2023

Signature of Alcohol Testing Program Staff Member

Date

Amendment

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: BROWARD COUNTY SO
Time of Inspection: 14:12

Date of Inspection: 02/01/2023

Serial Number: 80-007434
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 202112A Exp: 12/07/2023	0.08g/210L Test (g/210L) Lot#: 202206B Exp: 06/14/2024	0.20g/210L Test (g/210L) Lot#: 202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 402477283 Exp: 06/24/2025
/ 0.000	0.049	0.079	0.201	0.080
/ 0.000	0.049	0.079	0.201	0.079
/ 0.000	0.049	0.079	0.201	0.079

Number of Simulators Used: 5

Remarks:

00: Ambient Fail. JGUZMAN IN TRAINING

Ambient fail. unknown source. Turned on DA
TAN AND Repeated test without incident. 5/20/23

The above instrument complies (☒) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Signature and Printed Name

ANAYA S FRAZIER

02/01/2023
Date