



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Florida Highway Patrol

Instrument Serial Number: 80-006767

AGENCY INSPECTION DISCREPANCY

Agency Inspector: Taylor Ledford

Inspection Date: 01/15/2024

☐ A test was repeated without reason for repeat or the corrective action given

☐ Alcohol Free/Mouth Alcohol ☐ Alcohol Free Test ☐ Interferent Detect

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☐ Agency Inspection not conducted for calendar month

☐ Expired Alcohol Reference Solution or Dry Gas Standard was used for inspection

☐ 0.050 g/210L ☐ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Lot Number and/or Expiration Date for Standards entered incorrectly

☐ 0.050 g/210L ☒ 0.080 g/210L ☐ 0.200 g/210L ☐ 0.080 g/210L Dry Gas

☒ Other Electronic Data Review/Comments: The 0.08 ARS lot number is mistyped.

REQUESTED CORRECTIVE ACTION

☒ Record hand-written amendments on FDLE/ATP Form 40, initial and date amendments, mark report "AMENDED", and forward copy to Department Inspector

☐ Provide written explanation regarding referenced item(s) to Department Inspector

☐ Remove instrument from evidentiary use until otherwise directed by the Department

☐ Other:

Taylor Gutschow

Digitally signed by Taylor

Gutschow

Date: 2024.02.14 11:58:07 -05'00'

Signature of Alcohol Testing Program Staff Member

02/14/2024

Date

"Amended"

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL
Time of Inspection: 14:12

Date of Inspection: 01/15/2024

Serial Number: 80-006767
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:202303J Exp: 03/28/2025	0.08g/210L Test (g/210L) Lot#:202306C-07A Exp: 06/15/2024 7/11/2025	0.20g/210L Test (g/210L) Lot#:202206C Exp: 06/15/2024	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:402357111 Exp: 02/10/2025
0.000	0.049	0.079	0.200	0.079
0.000	0.049	0.079	0.200	0.078
0.000	0.050	0.079	0.201	0.079

Number of Simulators Used: 5

Remarks: Corrected the Lot # for 0.08 solution. (TL) 2/13/24
Corrected date on 0.08 solution. 7/11/2025. (TL) 2/21/24

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

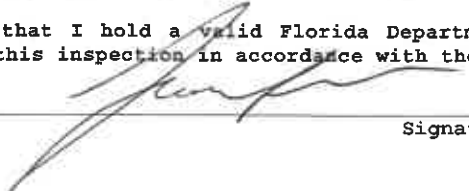

TAYLOR M LEDFORD

Signature and Printed Name

01/15/2024
Date