


LAB  
12/19/11

### January 2011 Update # 3 Control Tests Chart (All Control Tests)

Includes Control Tests Flagged Control Outside Tolerance (n=47), Interferent Detect (n=12) and RFI Detect (n=6)


subject  
provided breath during test  
sample control job

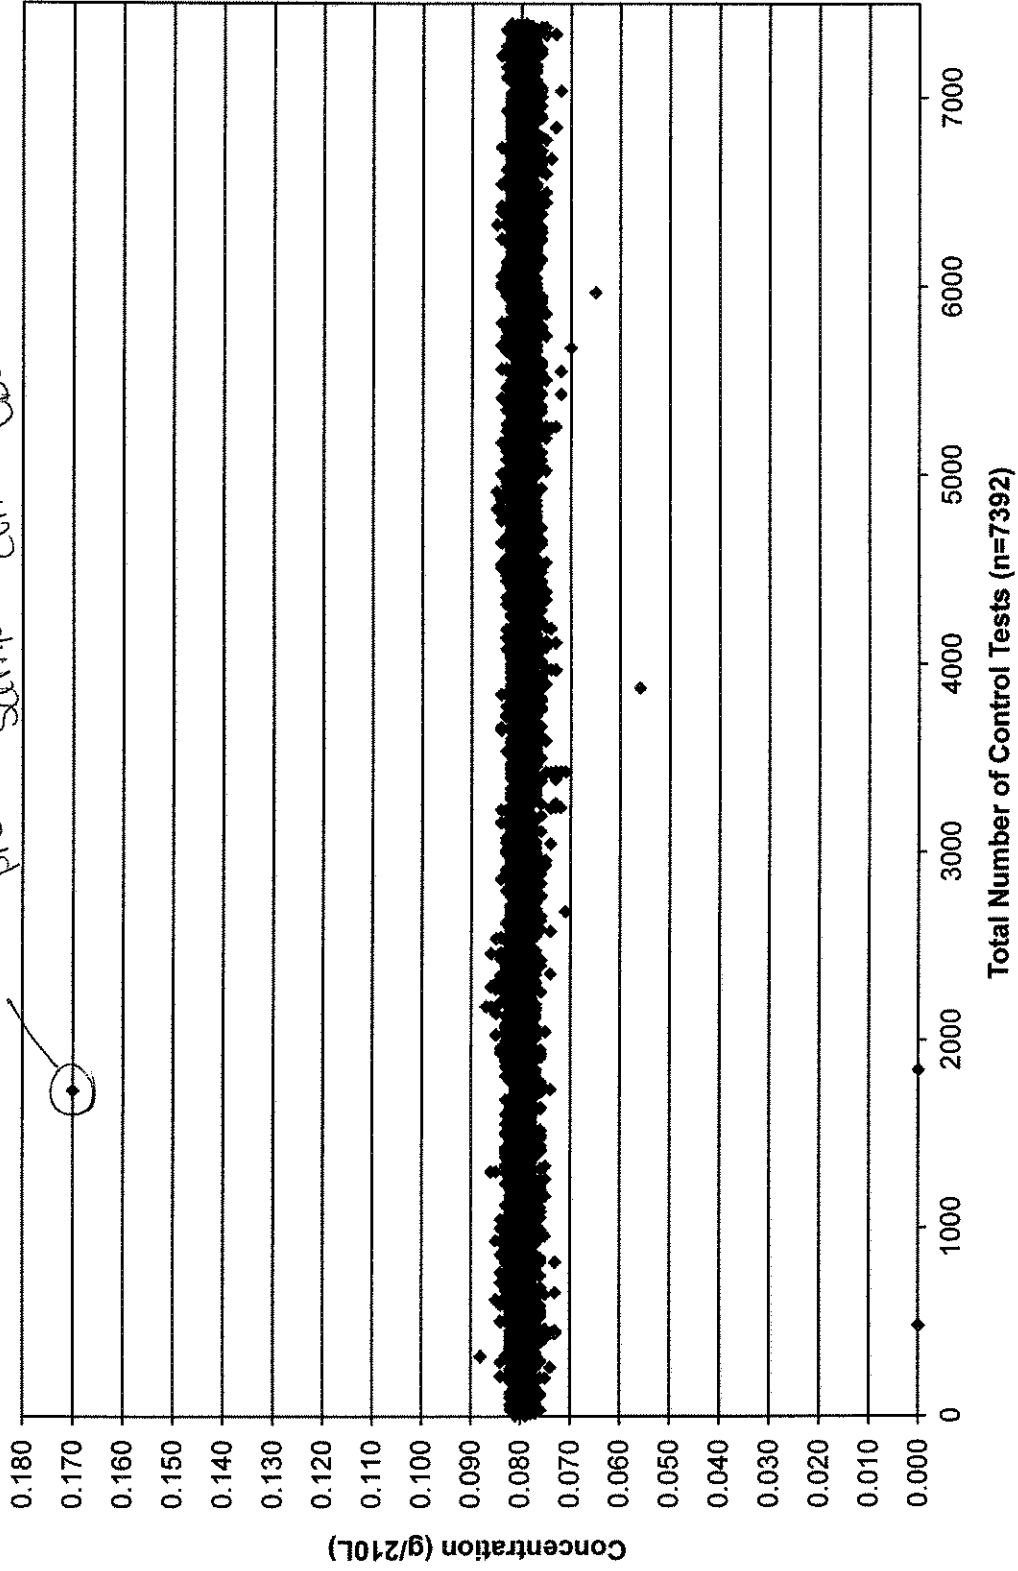

LAB  
12-11-11

### January 2011 Update # 3 Control Tests Flagged Control Outside Tolerance


subject provided breath sample during control test UDB

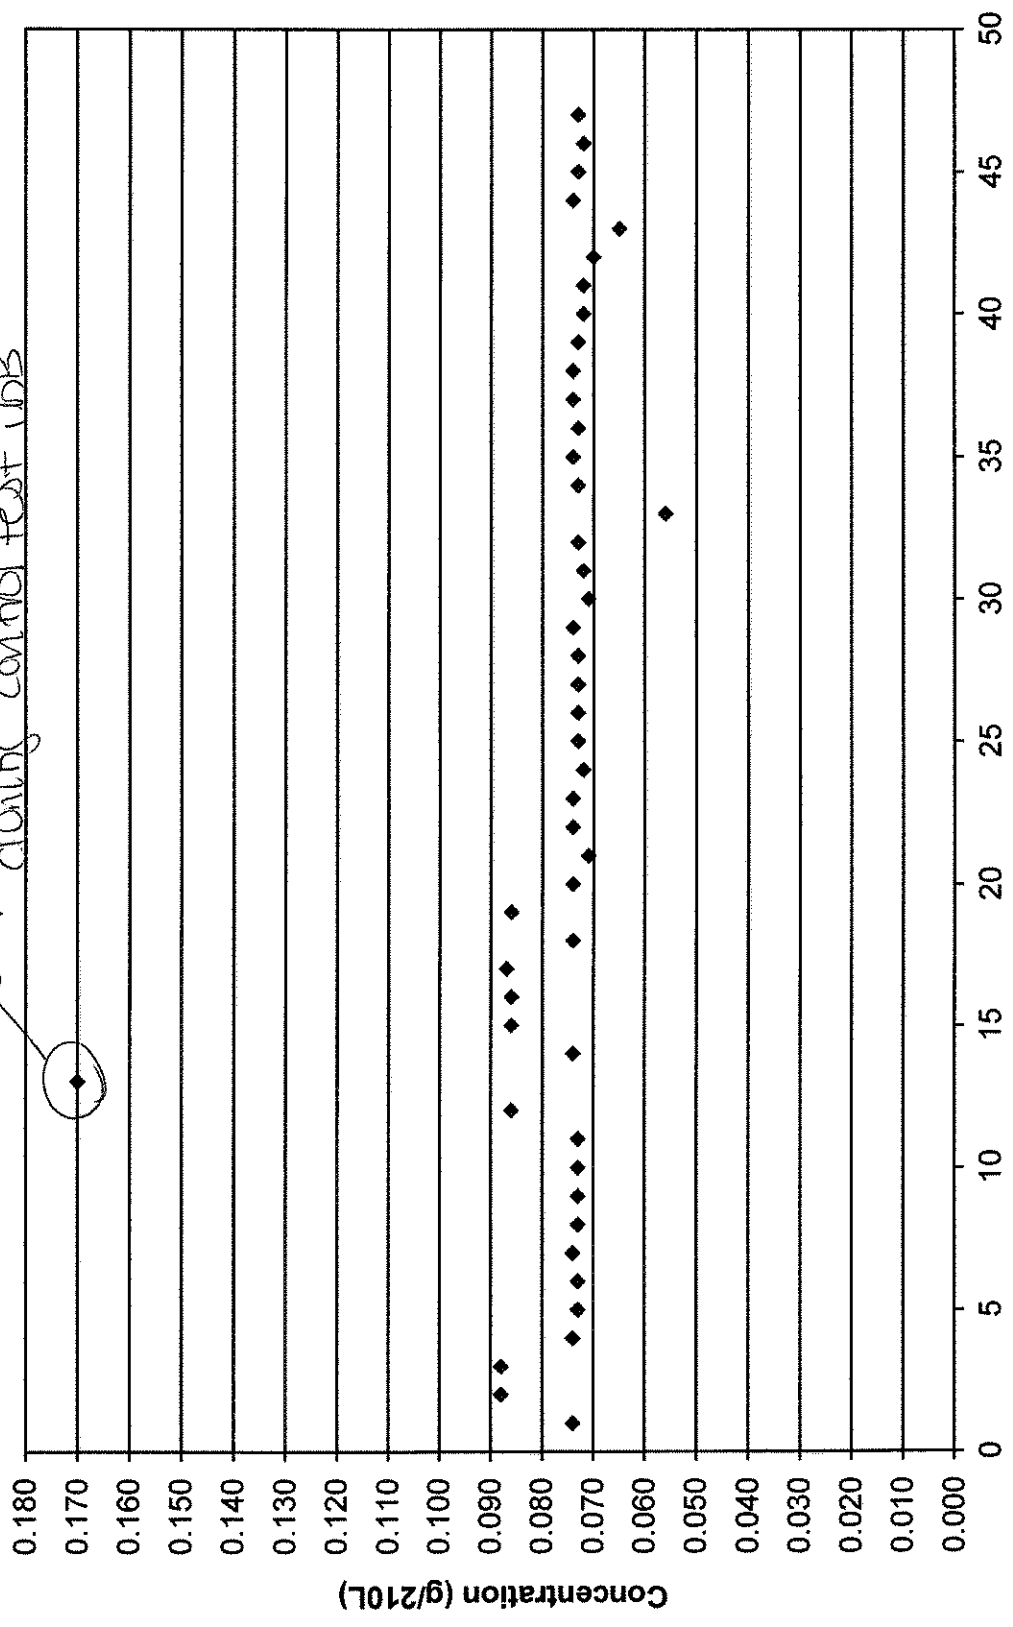

Total Number Flagged Control Outside Tolerance (n=47)


LAB  
12/19/11

### January 2011 Update # 3 Control Tests Flagged Interferent Detect

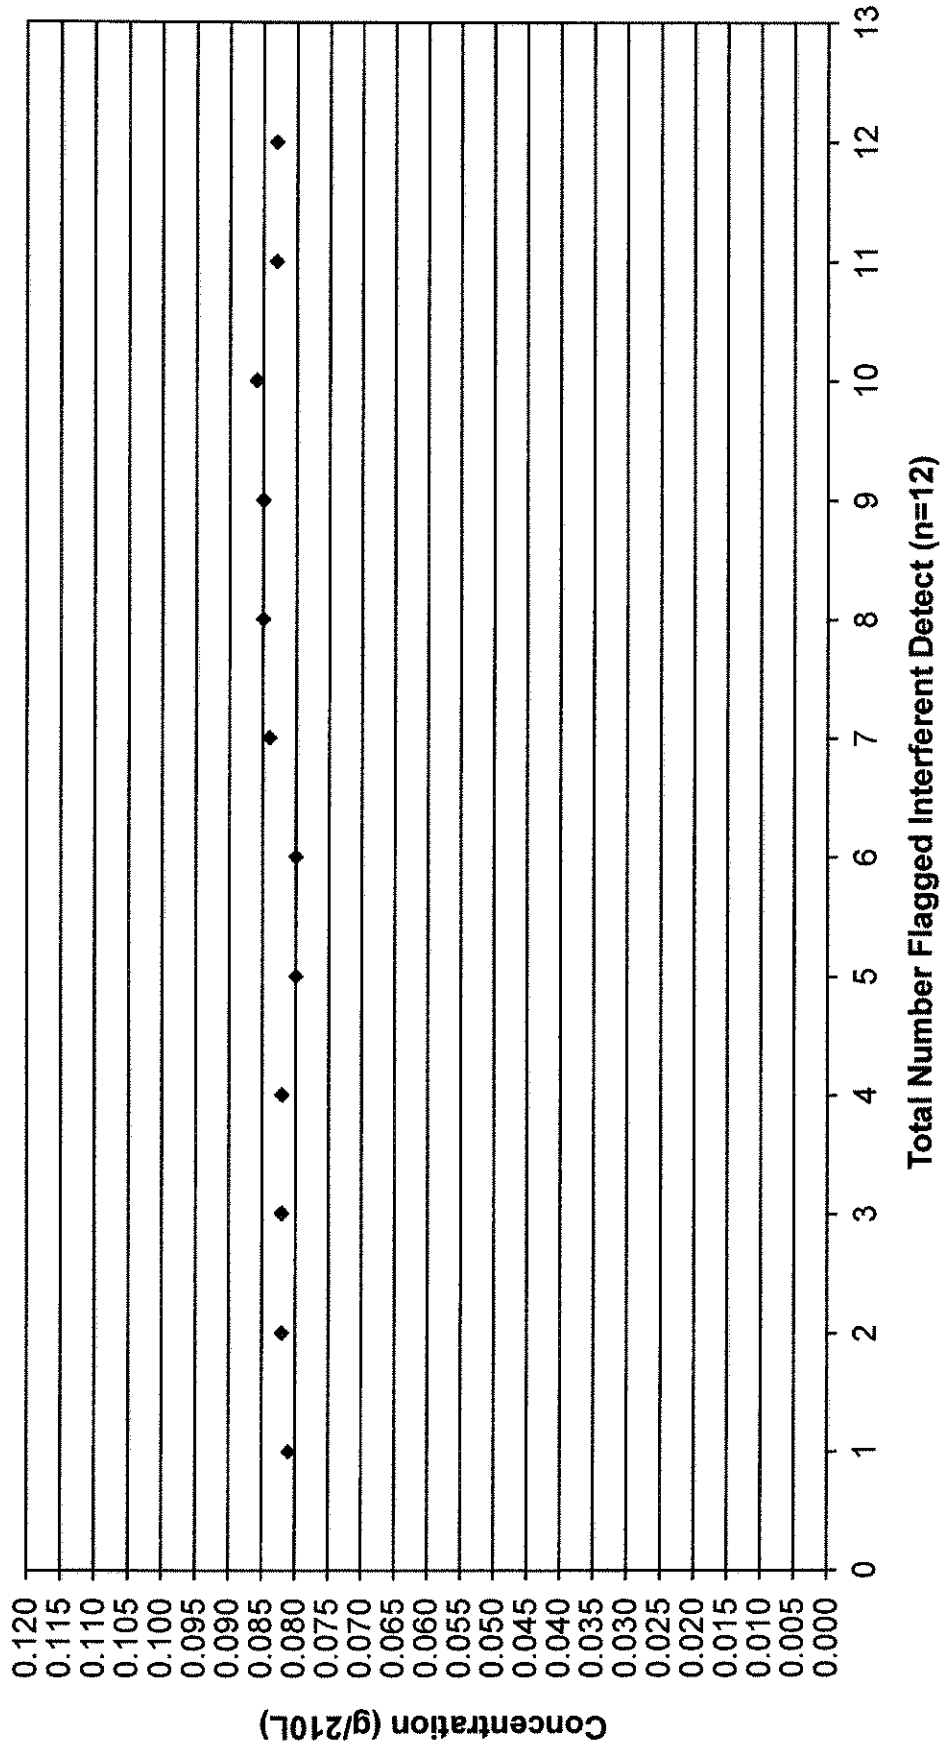

12/19/11  
WDB

### January 2011 Update # 3 Control Tests Flagged RFI Detect

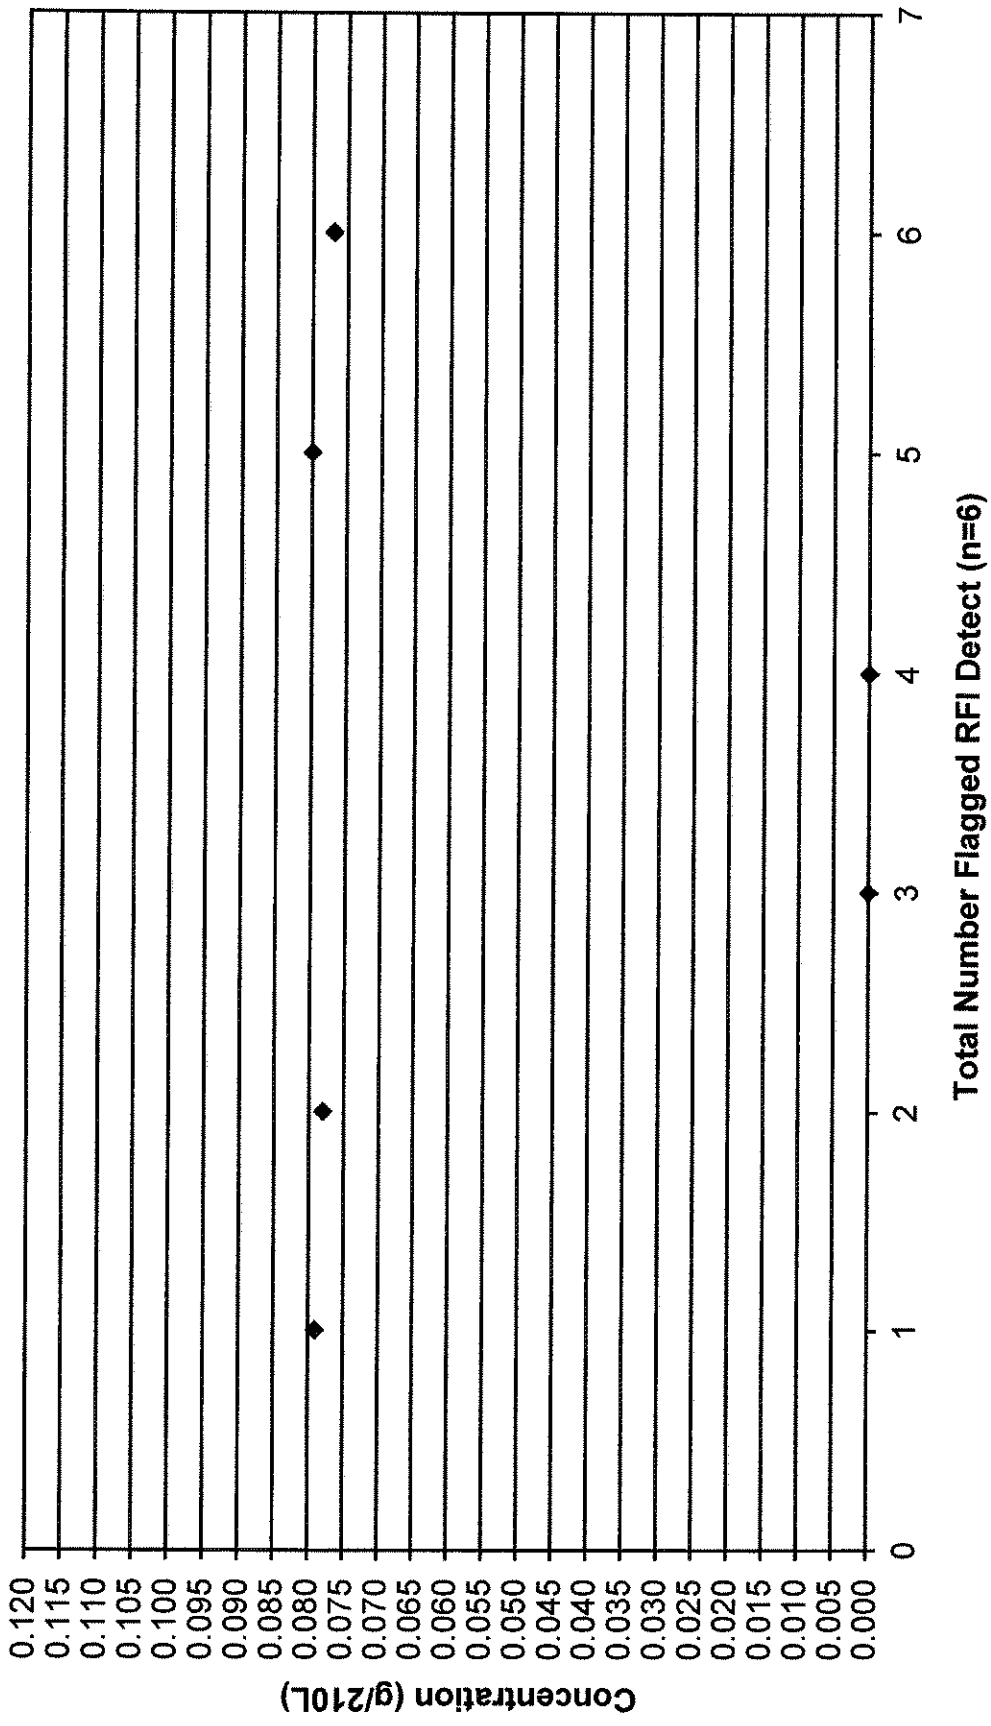

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001721

INSTRUMENT REGISTERED TO: PALM BAY P.D.  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: BADMAN, LIN, M  
BREATH TEST OPERATOR AGENCY: Palm Bay PD  
ARRESTING OFFICER: BADMAN, LIN  
ARRESTING OFFICER AGENCY: Palm Bay PD  
LAST AGENCY INSPECTION: 03/19/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 675059  
DRY GAS EXPIRY DATE: 09/25/2011  
VIOLATION CODE: DUI  
ARREST TIME: 16:56  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 17:07

SUBJECT'S LAST NAME: ROEMER

DATE/TIME OF TEST: 04/13/2011 17:48:40

---

Diagnostics Check	OK	17:47
Air Blank	0.000	17:47
Control Test	0.226	17:47
Air Blank	0.000	17:48

---

Control Outside Tolerance

*breath sample provided during control test  
COB*

---

Data Download Date/Time 04/23/2011 17:45

# Florida Department of Law Enforcement Alcohol Testing Program

## Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001721

INSTRUMENT REGISTERED TO: PALM BAY P.D.  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: BADMAN, LIN, M  
BREATH TEST OPERATOR AGENCY: Palm Bay PD  
ARRESTING OFFICER: BADMAN, LIN  
ARRESTING OFFICER AGENCY: Palm Bay PD  
LAST AGENCY INSPECTION: 03/19/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 675059  
DRY GAS EXPIRY DATE: 09/25/2011  
VIOLATION CODE: DUI  
ARREST TIME: 16:56  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 17:07

SUBJECT'S LAST NAME: ROEMER

DATE/TIME OF TEST: 04/13/2011 17:56:10

---

Diagnostics Check	OK	17:49
Air Blank	0.000	17:50
Control Test	0.079	17:50
Air Blank	0.000	17:51
Subject Sample #1	0.292	17:51
Breath Volume	2.695	17:51
Air Blank	0.000	17:52
Air Blank	0.000	17:54
Subject Sample #2	0.297	17:54
Breath Volume	2.714	17:54
Air Blank	0.000	17:55
Control Test	0.078	17:55
Air Blank	0.000	17:56
Diagnostics Check	OK	17:56

---

Data Download Date/Time 04/23/2011 17:45