


12-20-11

UDB


September 2011 Control Tests Chart (All Control Tests)

Includes Control Tests Flagged Control Outside Tolerance (n=68), Interferent Detect (n=9) and RFI Detect (n=2)

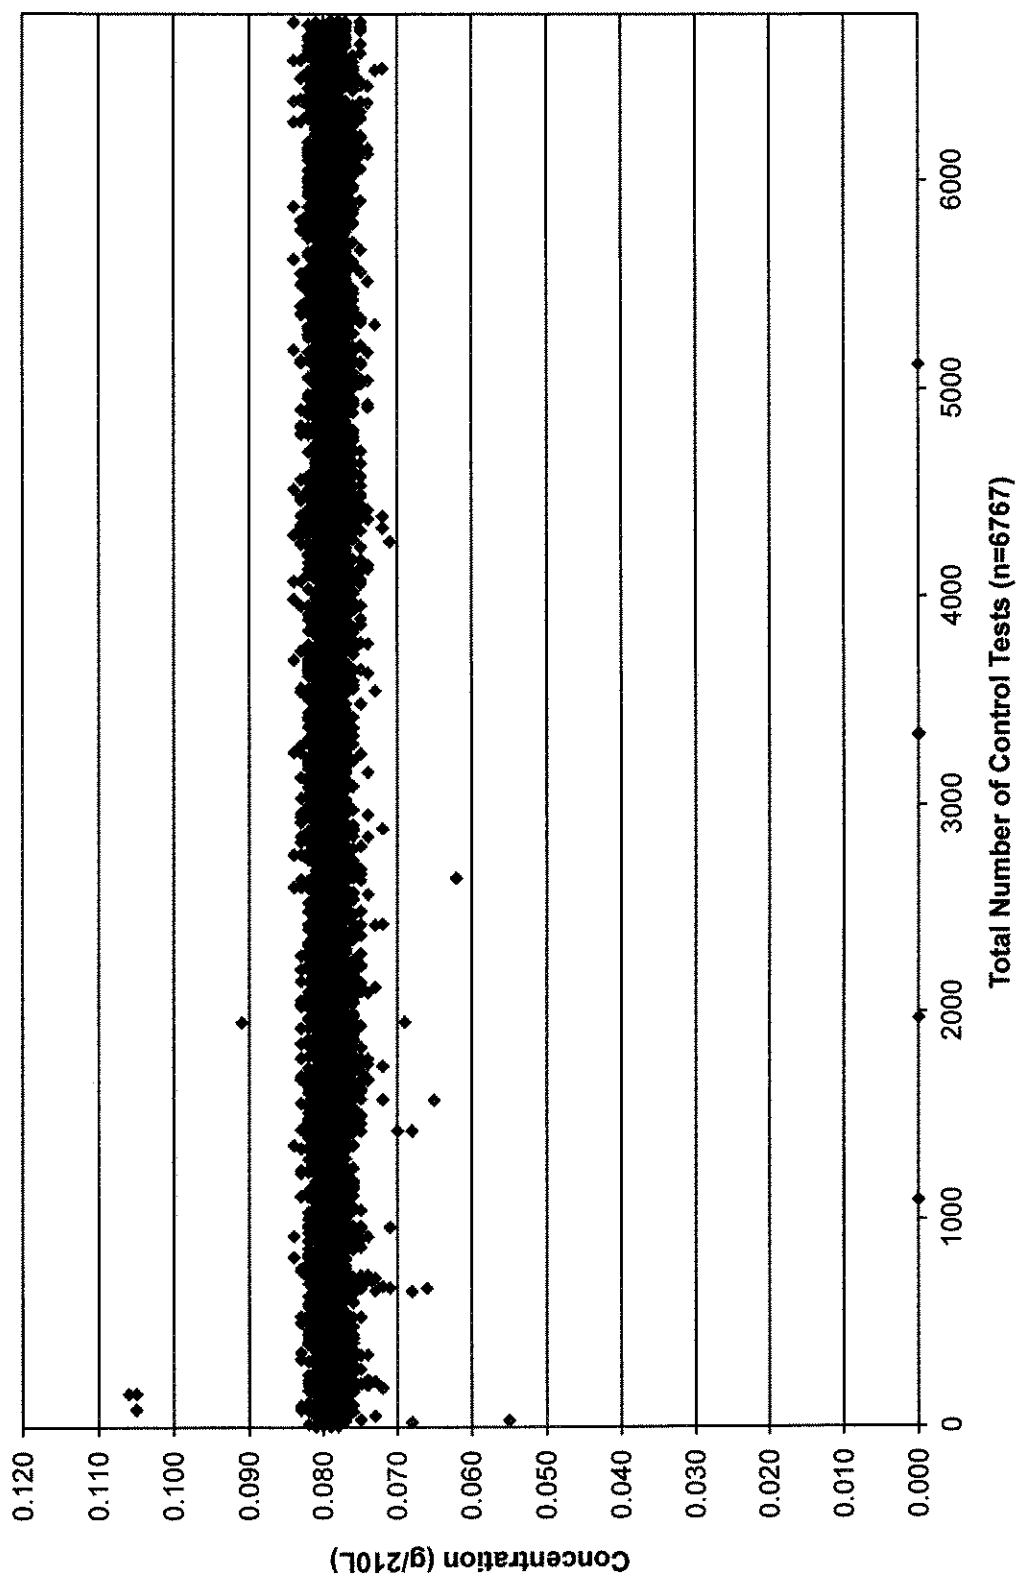


12-20-11
UD3

September 2011 Control Tests Flagged Control Outside Tolerance

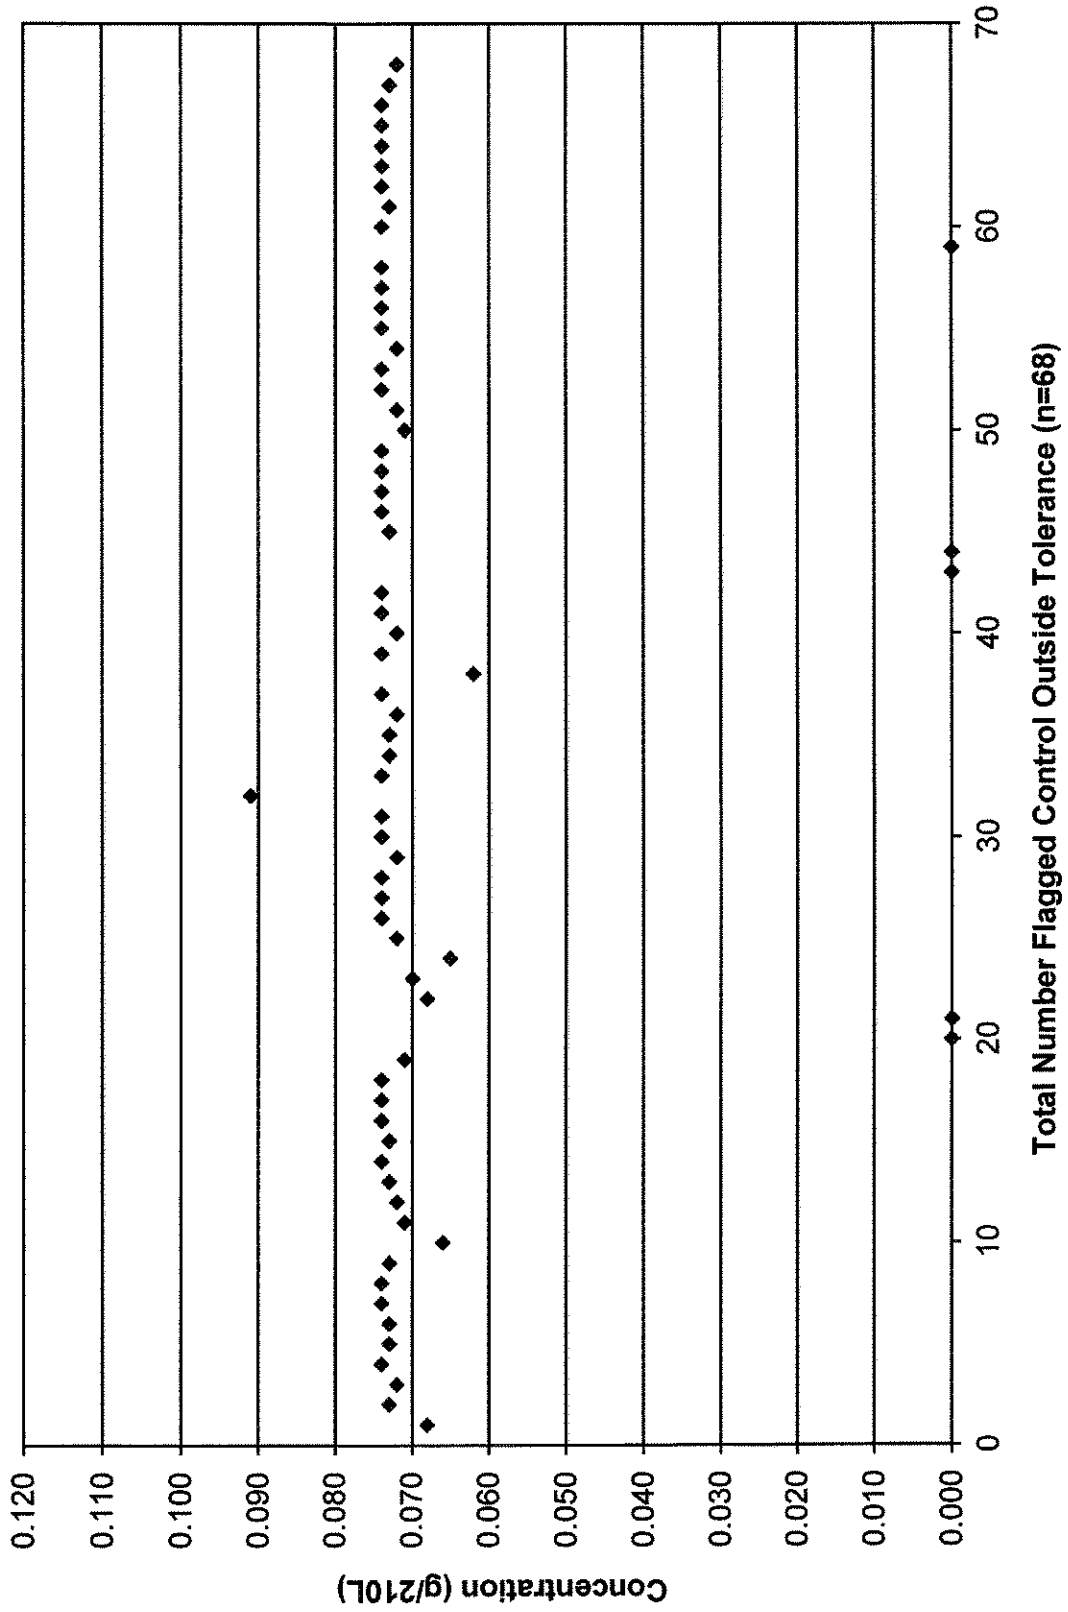


12-20-11
LDB

September 2011 Control Tests Flagged Interferent Detect

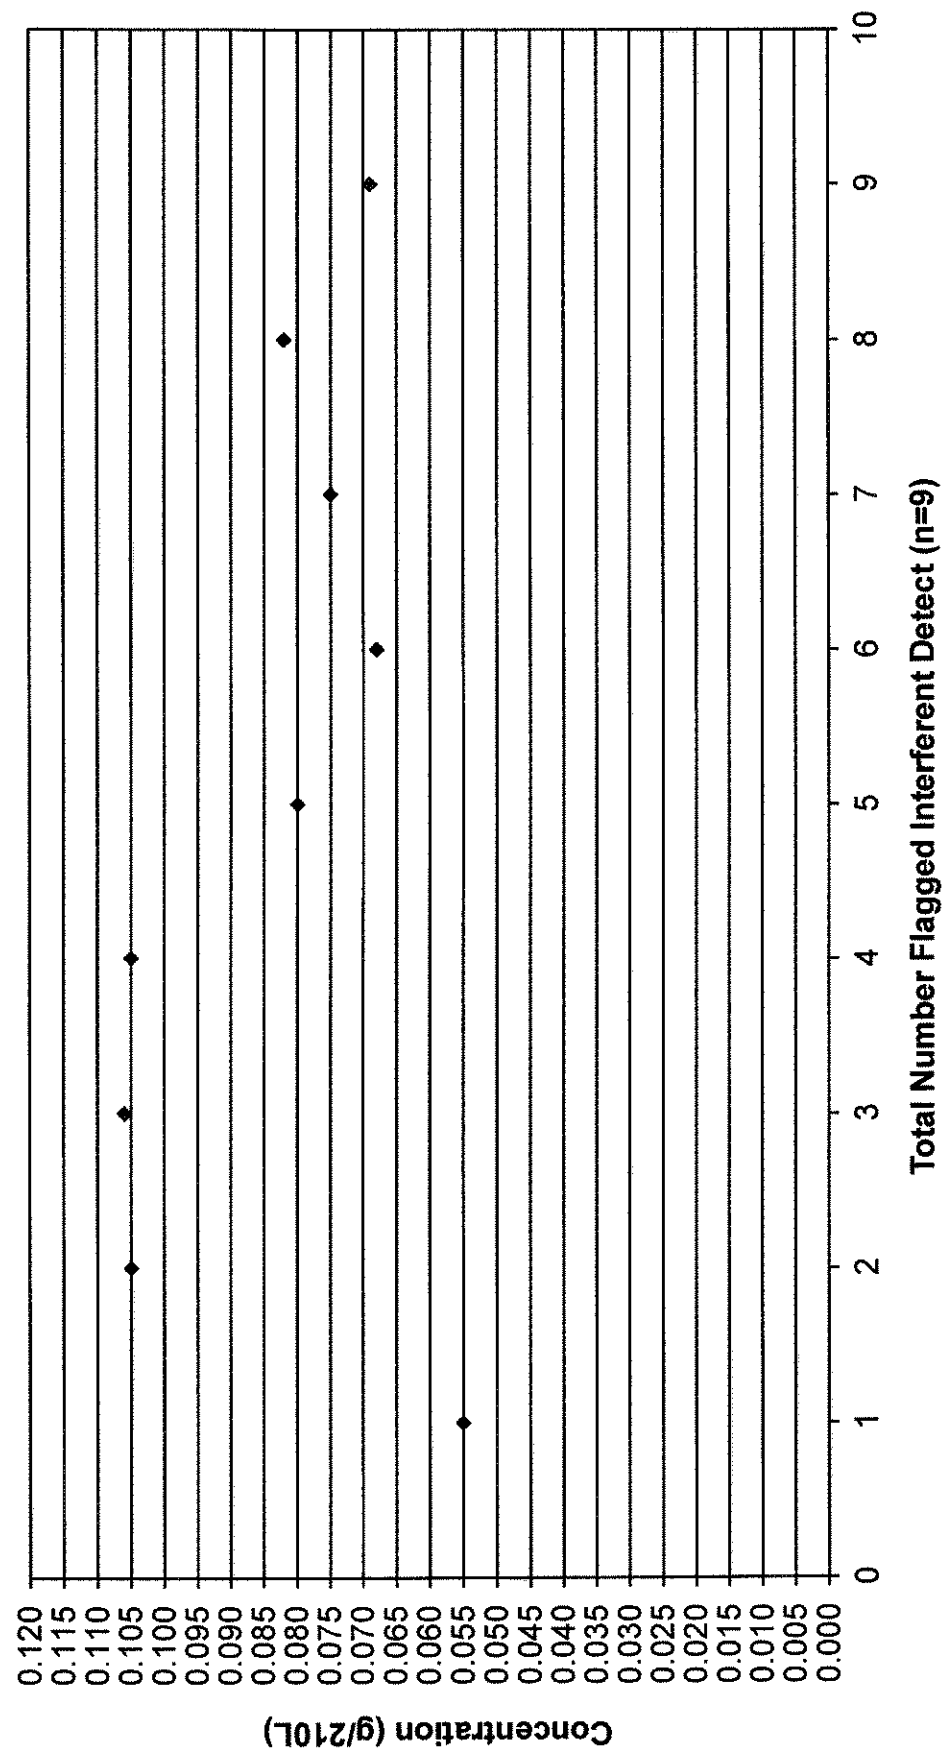

September 2011 Control Tests Flagged RFI Detect

12-20-11
UDB

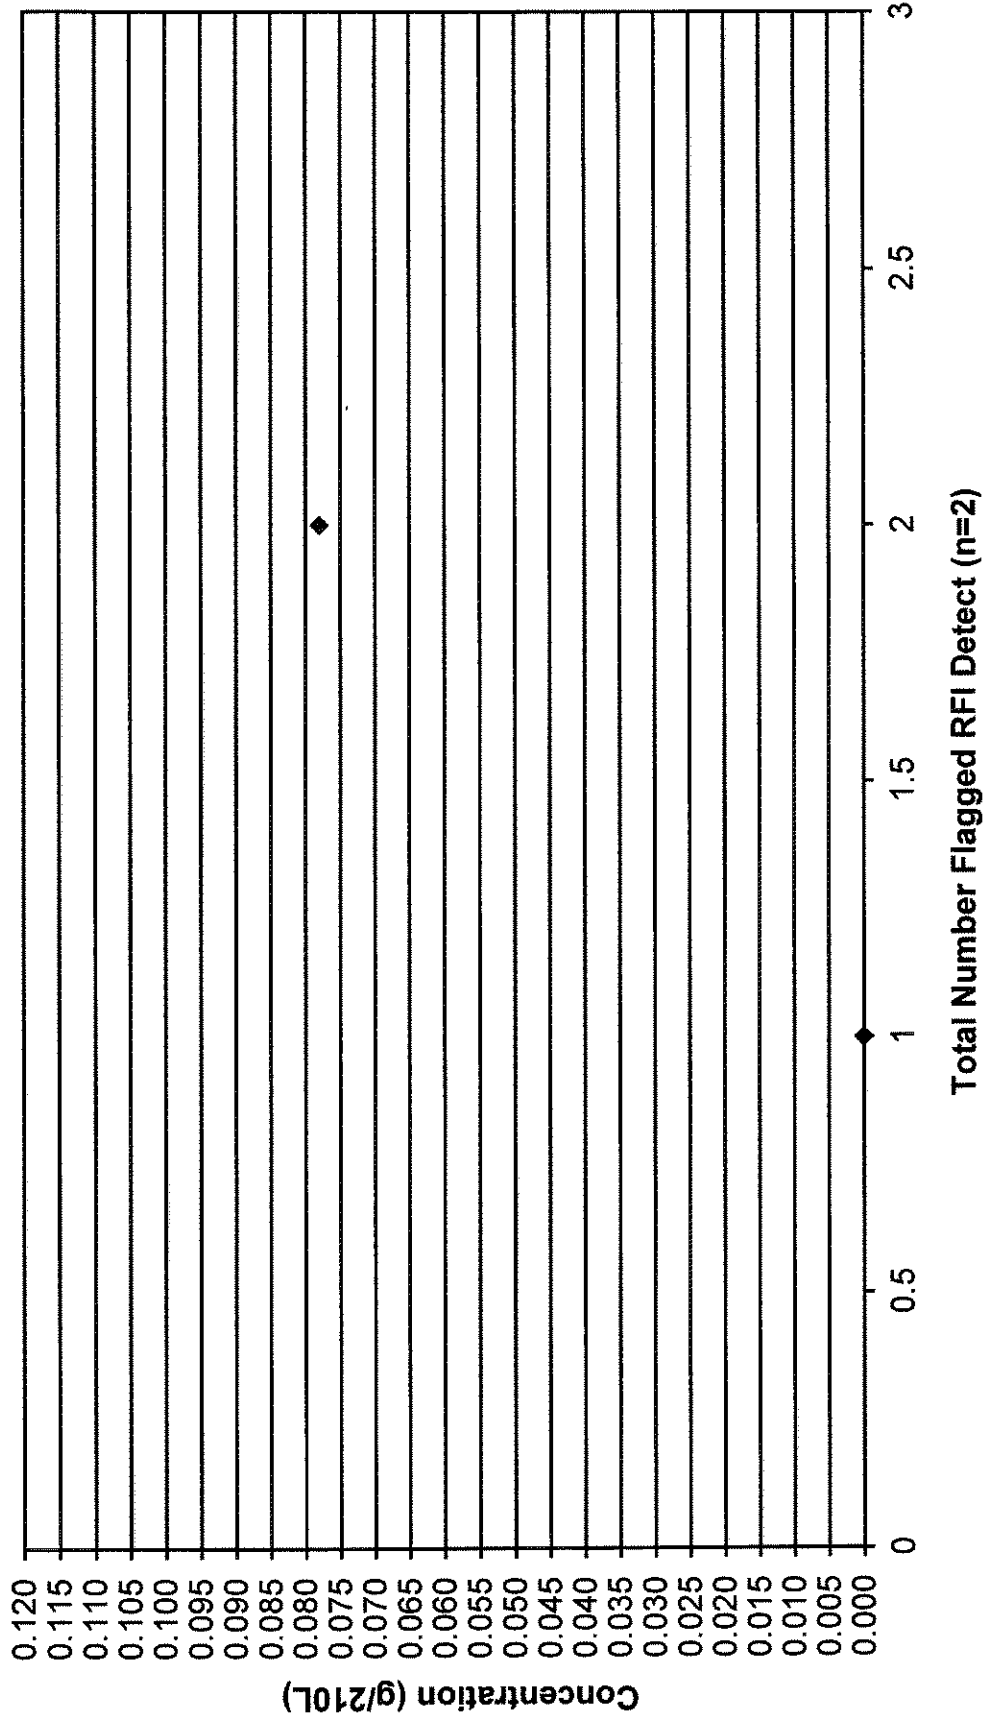

**Florida Department of Law Enforcement
Alcohol Testing Program**

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000884

INSTRUMENT REGISTERED TO: MIAMI-DADE PD
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: SLIMAK, M,
BREATH TEST OPERATOR AGENCY: Miami-Dade PD
ARRESTING OFFICER: SLIMAK, M
ARRESTING OFFICER AGENCY: Miami-Dade PD
LAST AGENCY INSPECTION: 09/02/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 03:12
GENDER: Male
OBSERVATION PERIOD BEGAN: 03:48

SUBJECT'S LAST NAME: FROMETA RODRIGUEZ

DATE/TIME OF TEST: 09/03/2011 04:22:38

Diagnostics Check	OK	04:21	
Air Blank	0.000	04:21	
Control Test	0.105	04:22	Interferent Detect
Air Blank	0.000	04:22	

Data Download Date/Time 10/13/2011 13:00

Florida Department of Law Enforcement Alcohol Testing Program

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000884

INSTRUMENT REGISTERED TO: MIAMI-DADE PD
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: SUAREZ, CARLOS, A
BREATH TEST OPERATOR AGENCY: Miami-Dade PD
ARRESTING OFFICER: SUAREZ, CARLOS
ARRESTING OFFICER AGENCY: Miami-Dade PD
LAST AGENCY INSPECTION: 09/02/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 05:28
GENDER: Male
OBSERVATION PERIOD BEGAN: 06:12

SUBJECT'S LAST NAME: MARTINEZ

DATE/TIME OF TEST: 09/03/2011 06:34:51

Diagnostics Check	OK	06:33	
Air Blank	0.000	06:33	
Control Test	0.106	06:34	Interferent Detect
Air Blank	0.000	06:34	

Data Download Date/Time 10/13/2011 13:00

**Florida Department of Law Enforcement
Alcohol Testing Program**

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000884

INSTRUMENT REGISTERED TO: MIAMI-DADE PD
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: SUAREZ, CARLOS, A
BREATH TEST OPERATOR AGENCY: Miami-Dade PD
ARRESTING OFFICER: SUAREZ, CARLOS
ARRESTING OFFICER AGENCY: Miami-Dade PD
LAST AGENCY INSPECTION: 09/02/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 05:28
GENDER: Male
OBSERVATION PERIOD BEGAN: 06:12

SUBJECT'S LAST NAME: MARTINEZ

DATE/TIME OF TEST: 09/03/2011 06:37:48

Diagnostics Check	OK	06:36	
Air Blank	0.000	06:36	
Control Test	0.105	06:37	Interferent Detect
Air Blank	0.000	06:37	

Data Download Date/Time 10/13/2011 13:00