


August 2011 Updated Control Tests Chart (All Control Tests)

Includes Control Tests Flagged Control Outside Tolerance (n=69), Interferent Detect (n=13) and RFI Detect (n=3)

12-20-11

LOB

Breath samples provided during control test
LOB

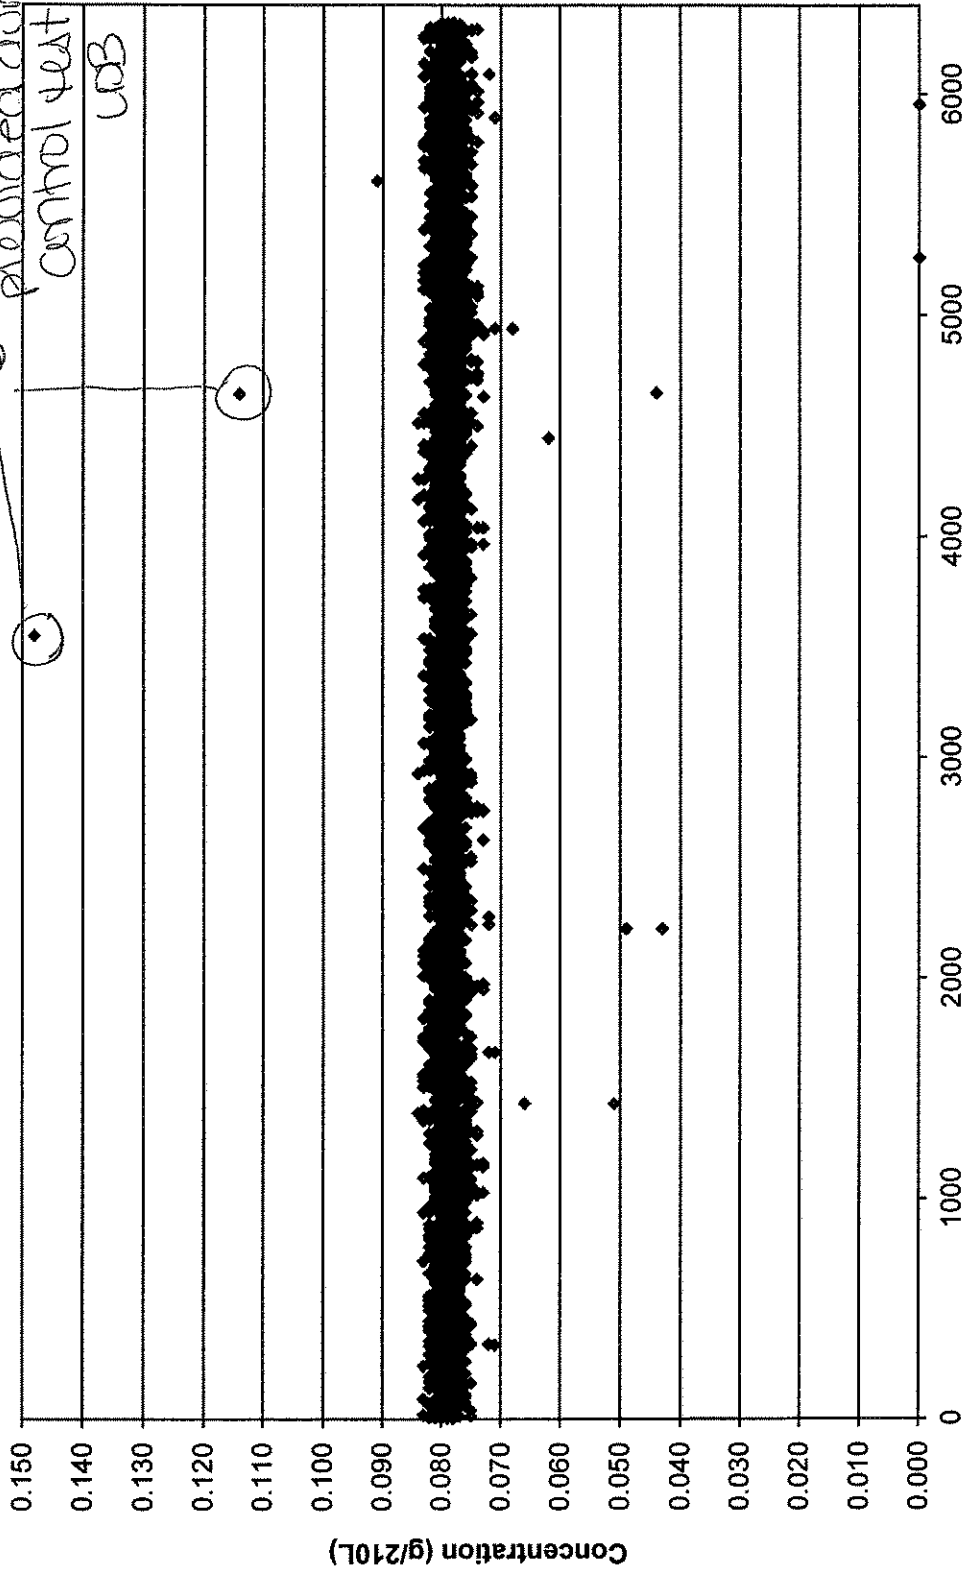


Total Number of Control Tests (n=6321)

12-20-11
DOB

August 2011 Updated Control Tests Flagged Control Outside Tolerance

⊙ Subject provided
breast sample
during control test
LOB

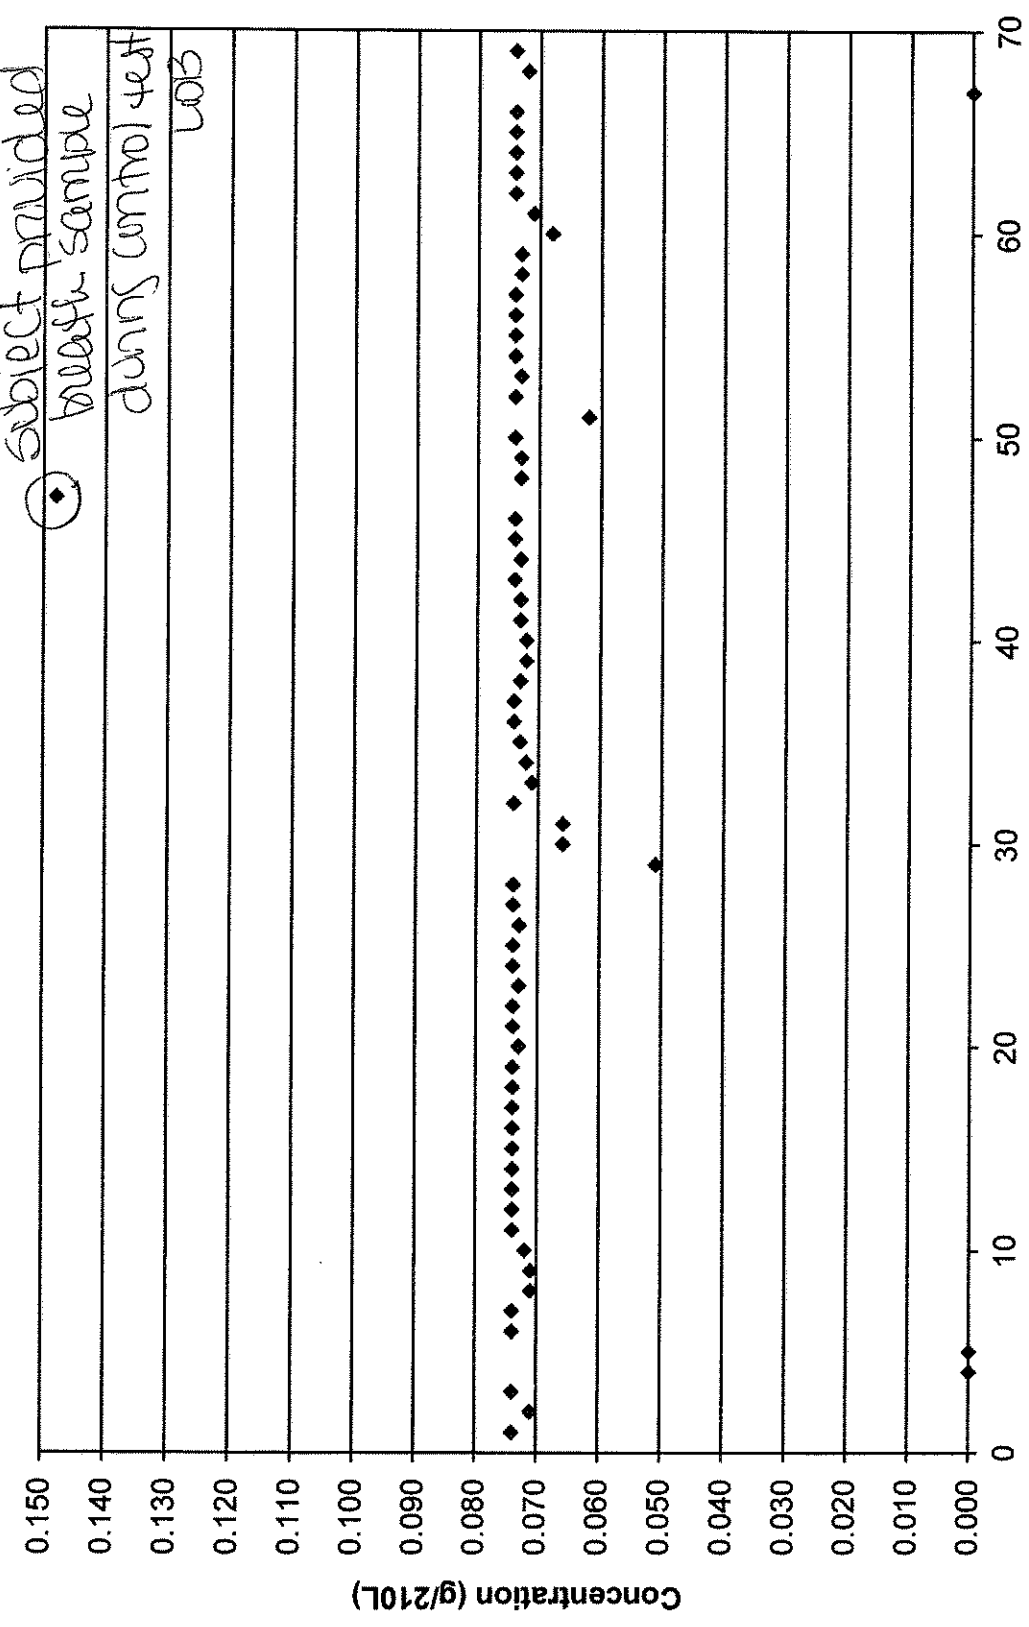


Total Number Flagged Control Outside Tolerance (n=69)

August 2011 Updated Control Tests Flagged Interferent Detect

12-20-11
LAB


breath sample provided
during control test
LAB

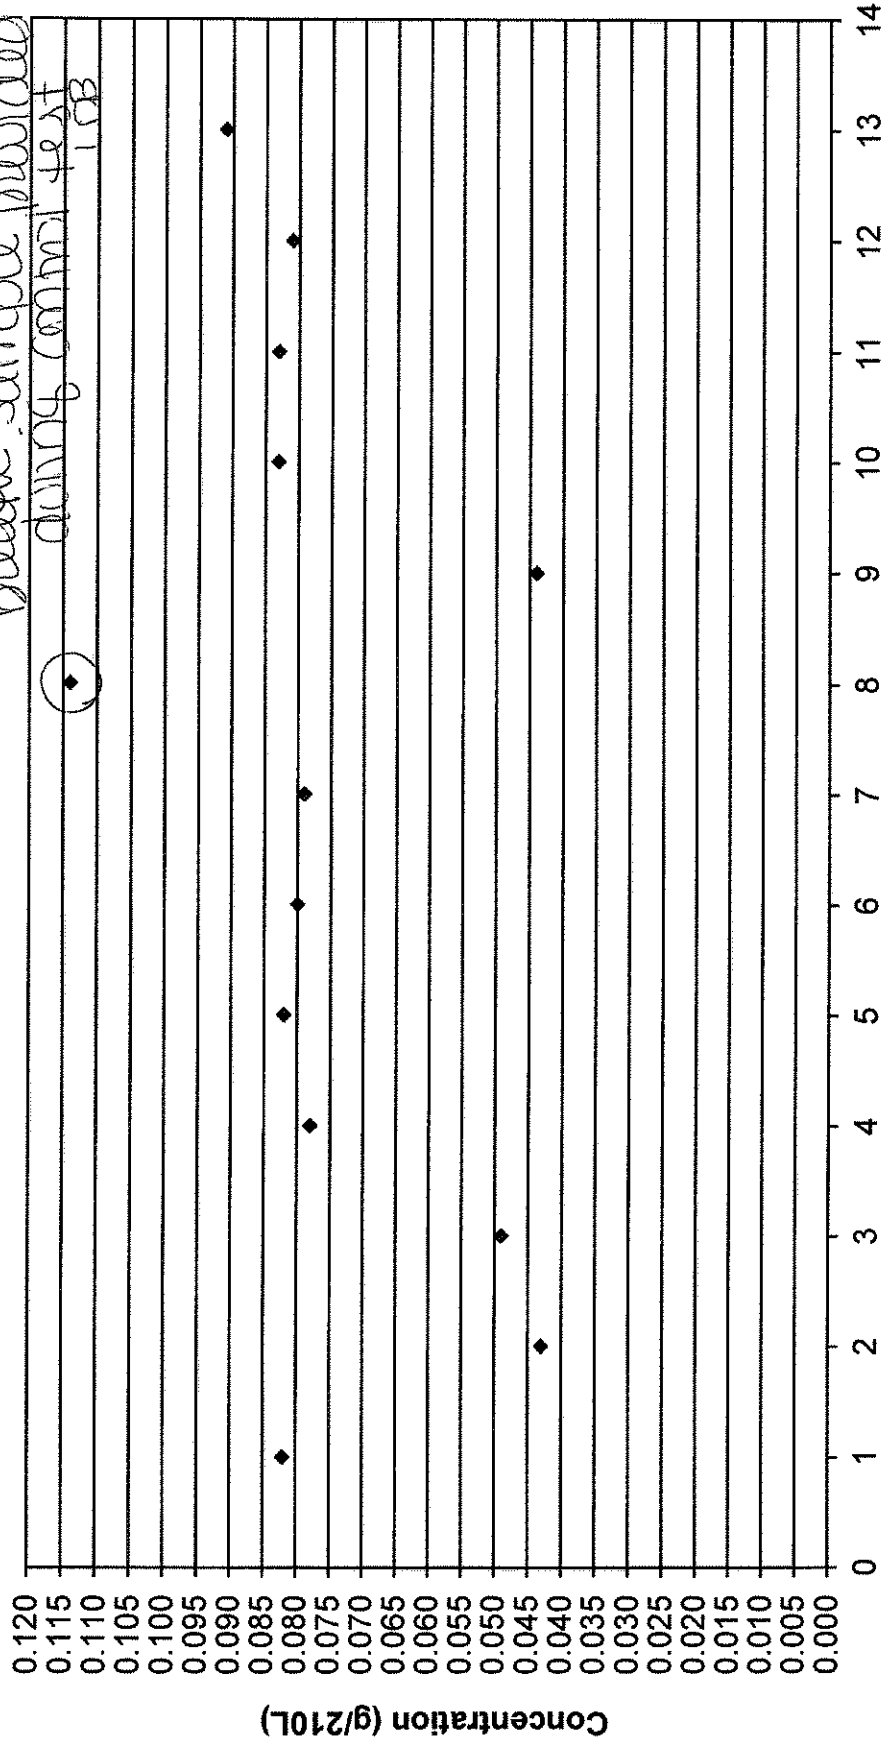

Total Number Flagged Interferent Detect (n=13)

August 2011 Updated Control Tests Flagged RFI Detect

12-20-11
VDB

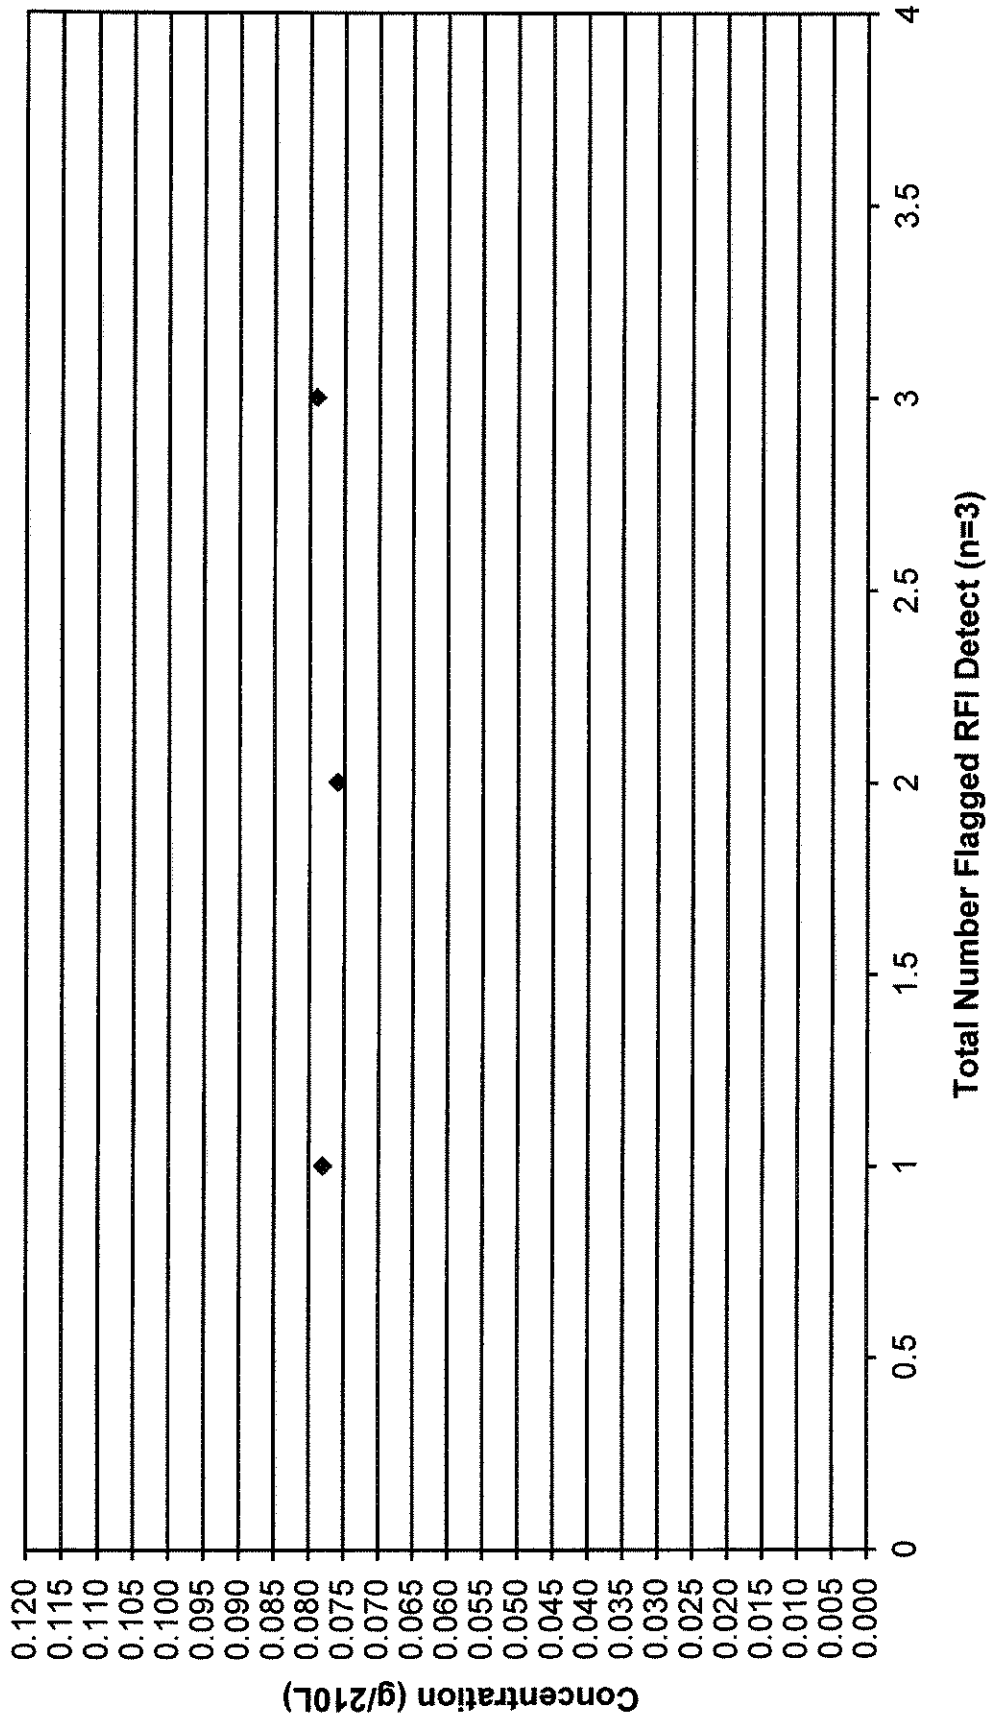

**Florida Department of Law Enforcement
Alcohol Testing Program**

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000942

INSTRUMENT REGISTERED TO: COLLIER COUNTY SO
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: PEABODY, MICHAEL, F
BREATH TEST OPERATOR AGENCY: Collier County SO
ARRESTING OFFICER: HINCHLIFFE, GREG
ARRESTING OFFICER AGENCY: Collier County SO
LAST AGENCY INSPECTION: 08/01/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 13811080A1
DRY GAS EXPIRY DATE: 07/01/2013
VIOLATION CODE: DUI
ARREST TIME: 23:57
GENDER: Female
OBSERVATION PERIOD BEGAN: 23:57

SUBJECT'S LAST NAME: BOURQUE

DATE/TIME OF TEST: 08/21/2011 00:20:51

Diagnostics Check	OK	00:19	
Air Blank	0.000	00:19	
Control Test	0.148	00:20	Control Outside Tolerance
Air Blank	0.000	00:20	

Data Download Date/Time 09/01/2011 16:03

— breath
sample
provided
during
control
test
LOB

**Florida Department of Law Enforcement
Alcohol Testing Program**

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000942

INSTRUMENT REGISTERED TO: COLLIER COUNTY SO
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: PEABODY, MICHAEL, F
BREATH TEST OPERATOR AGENCY: Collier County SO
ARRESTING OFFICER: HINCHLIFFE, GREGG
ARRESTING OFFICER AGENCY: Collier County SO
LAST AGENCY INSPECTION: 08/01/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 13811080A1
DRY GAS EXPIRY DATE: 07/01/2013
VIOLATION CODE: DUI
ARREST TIME: 23:57
GENDER: Female
OBSERVATION PERIOD BEGAN: 23:57

SUBJECT'S LAST NAME: ~~89234~~ **BOURQUE** *LOB*

DATE/TIME OF TEST: 08/21/2011 00:30:53

Diagnostics Check	OK	00:24
Air Blank	0.000	00:25
Control Test	0.078	00:25
Air Blank	0.000	00:26
Subject Sample #1	0.159	00:26
Breath Volume	2.039	00:26
Air Blank	0.000	00:27
Air Blank	0.000	00:28
Subject Sample #2	0.161	00:29
Breath Volume	1.367	00:29
Air Blank	0.000	00:29
Control Test	0.078	00:30
Air Blank	0.000	00:30
Diagnostics Check	OK	00:30

Data Download Date/Time 09/01/2011 16:03

**Florida Department of Law Enforcement
Alcohol Testing Program**

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001742

INSTRUMENT REGISTERED TO: MANATEE COUNTY SO
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: CLINE, GLENN, A
BREATH TEST OPERATOR AGENCY: Manatee County SO
ARRESTING OFFICER: VAUGHN, RYAN
ARRESTING OFFICER AGENCY: Bradenton PD
LAST AGENCY INSPECTION: 08/17/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 23:11
GENDER: Female
OBSERVATION PERIOD BEGAN: 23:44

SUBJECT'S LAST NAME: WHITTAKER

DATE/TIME OF TEST: 08/27/2011 00:13:41

Diagnostics Check	OK	00:07	
Air Blank	0.000	00:07	
Control Test	0.079	00:07	
Air Blank	0.000	00:08	
Subject Sample #1	0.183	00:08	
Breath Volume	2.234	00:08	
Air Blank	0.000	00:09	
Air Blank	0.000	00:11	
Subject Sample #2	0.172	00:11	
Breath Volume	2.011	00:11	
Air Blank	0.000	00:12	
Control Test	0.114	00:12	Interferent Detect
Air Blank		00:13	Purge Fail

*Breath sample during control test.
WOB*

Data Download Date/Time 10/11/2011 14:44

Florida Department of Law Enforcement Alcohol Testing Program

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001742

INSTRUMENT REGISTERED TO: MANATEE COUNTY SO
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: CLINE, GLENN, A
BREATH TEST OPERATOR AGENCY: Manatee County SO
ARRESTING OFFICER: VAUGHN, RYAN
ARRESTING OFFICER AGENCY: Bradenton PD
LAST AGENCY INSPECTION: 08/17/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 23:11
GENDER: Female
OBSERVATION PERIOD BEGAN: 23:44

SUBJECT'S LAST NAME: WHITTAKER

DATE/TIME OF TEST: 08/27/2011 00:18:39

Diagnostics Check	OK	00:15	
Air Blank	0.000	00:15	
Control Test	0.079	00:16	
Air Blank	0.000	00:16	
Subject Sample #1		00:17	Interferent Detect
Breath Volume	2.460	00:17	
Air Blank	0.000	00:17	
Control Test	0.044	00:18	Interferent Detect
Air Blank	0.000	00:18	

Data Download Date/Time 10/11/2011 14:44

Florida Department of Law Enforcement Alcohol Testing Program

Subject Test Electronic Data

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001742

INSTRUMENT REGISTERED TO: MANATEE COUNTY SO
SOFTWARE VERSION: 8100.27
BREATH TEST OPERATOR: CLINE, GLENN, A
BREATH TEST OPERATOR AGENCY: Manatee County SO
ARRESTING OFFICER: VAUGHN, RYAN
ARRESTING OFFICER AGENCY: Bradenton PD
LAST AGENCY INSPECTION: 08/17/2011

Date or Time Changed: No
DRY GAS STANDARD LOT #: 885290
DRY GAS EXPIRY DATE: 10/19/2012
VIOLATION CODE: DUI
ARREST TIME: 23:11
GENDER: Female
OBSERVATION PERIOD BEGAN: 23:44

SUBJECT'S LAST NAME: WHITTAKER

DATE/TIME OF TEST: 08/27/2011 00:26:01

Diagnostics Check	OK	00:19
Air Blank	0.000	00:20
Control Test	0.079	00:20
Air Blank	0.000	00:21
Subject Sample #1	0.169	00:21
Breath Volume	1.625	00:21
Air Blank	0.000	00:22
Air Blank	0.000	00:24
Subject Sample #2	0.171	00:24
Breath Volume	1.945	00:24
Air Blank	0.000	00:25
Control Test	0.078	00:25
Air Blank	0.000	00:25
Diagnostics Check	OK	00:26

Data Download Date/Time 10/11/2011 14:44