


# February 2011 Updated Control Tests Chart (All Control Tests)

updated  
02-22-11

Includes Control Tests Flagged Control Outside Tolerance (n=56), Interferent Detect (n=12) and RFI Detect (n=5)


breath sample provided during control test (DOB)

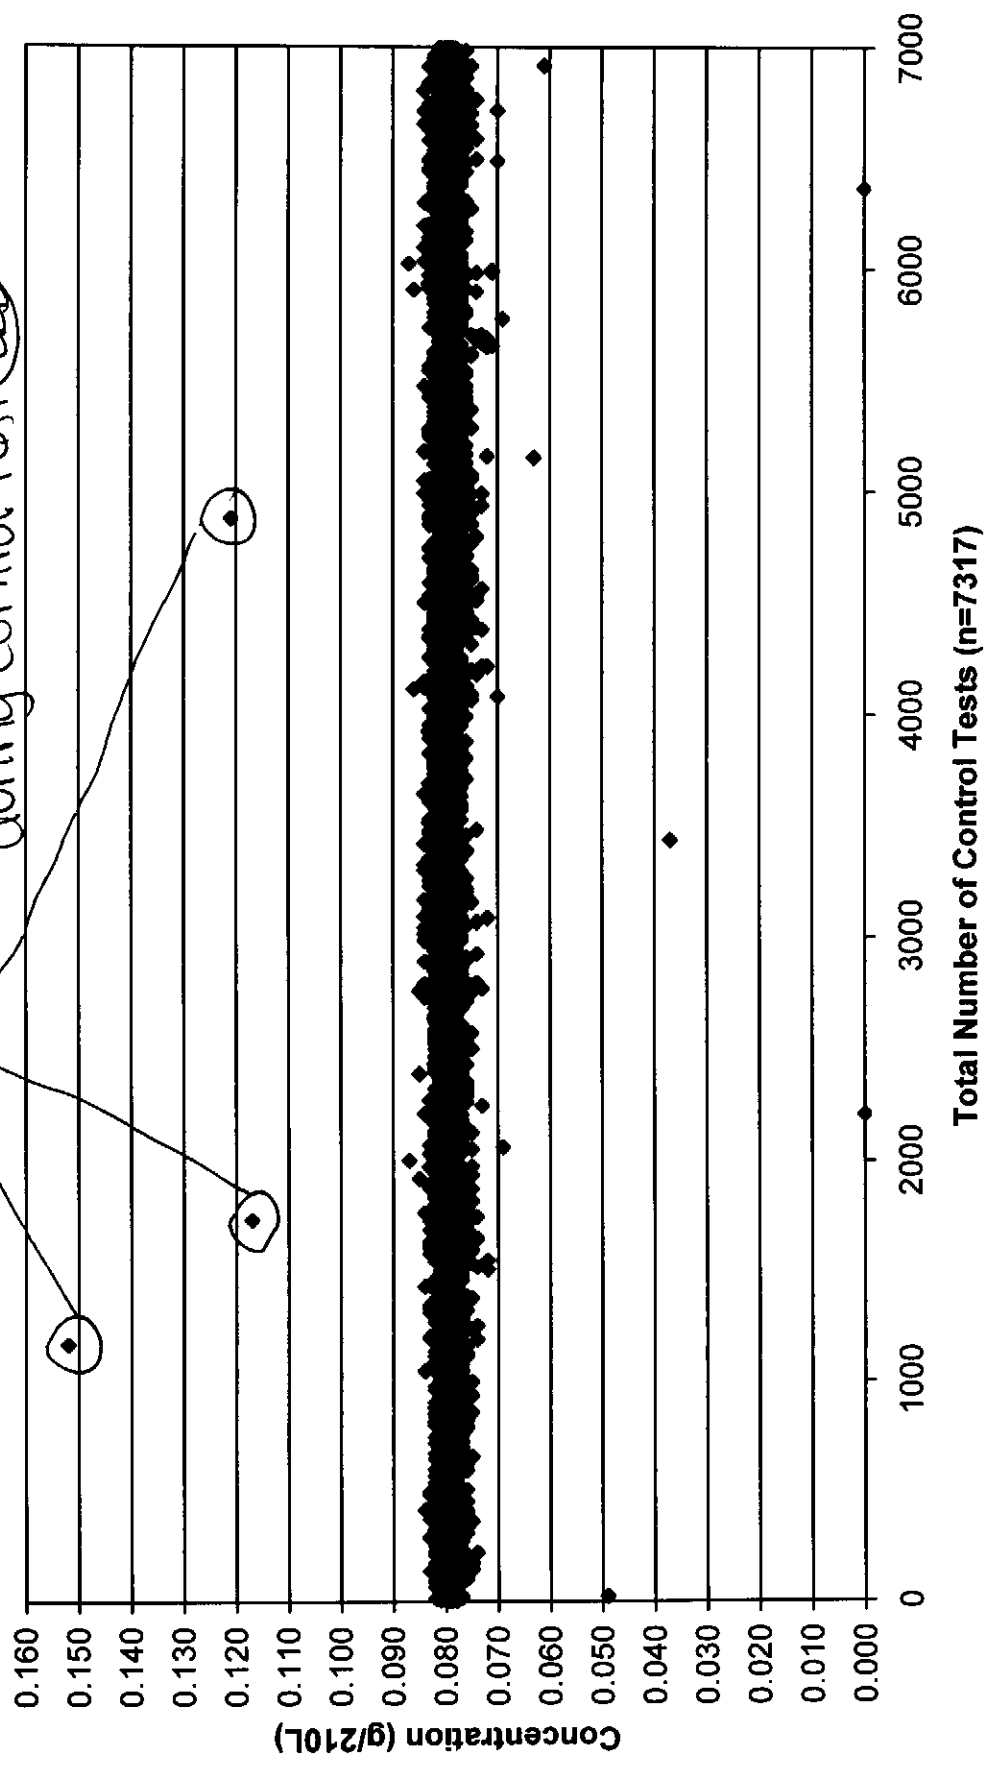

# February 2011 Updated Control Tests Flagged Control Outside Tolerance


Updated  
6/22/11  
UAS

subject provided breath sample during control test

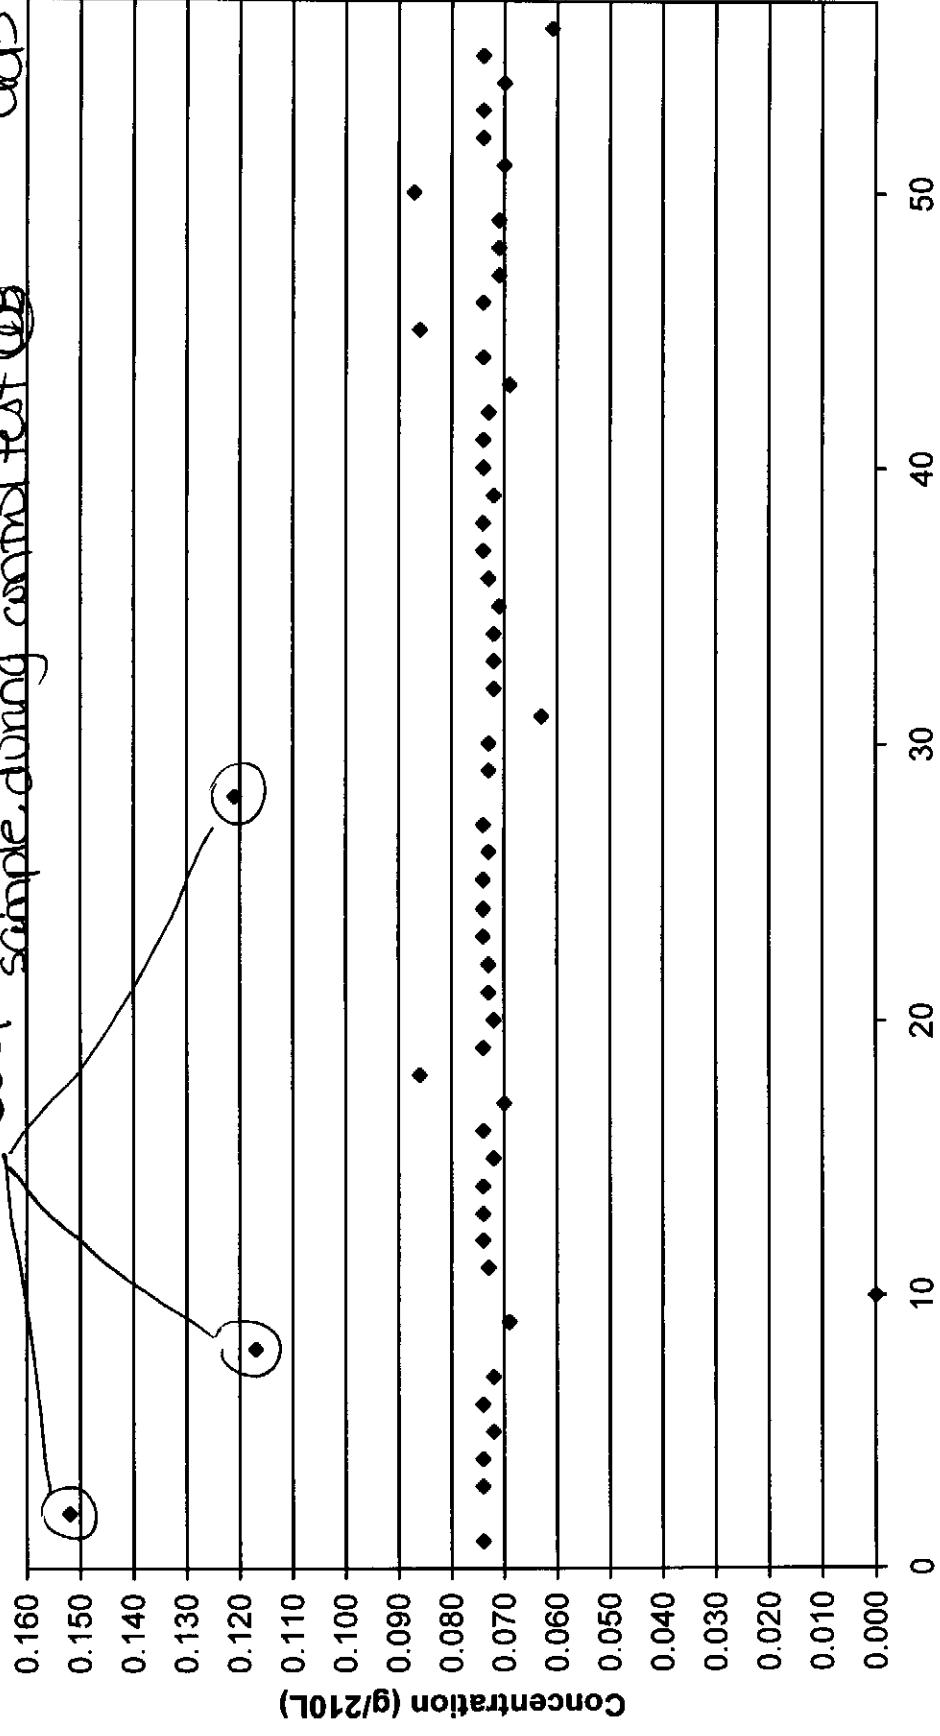


Updated  
10-22-11  
JOB

### February 2011 Updated Control Tests Flagged Interferent Detect

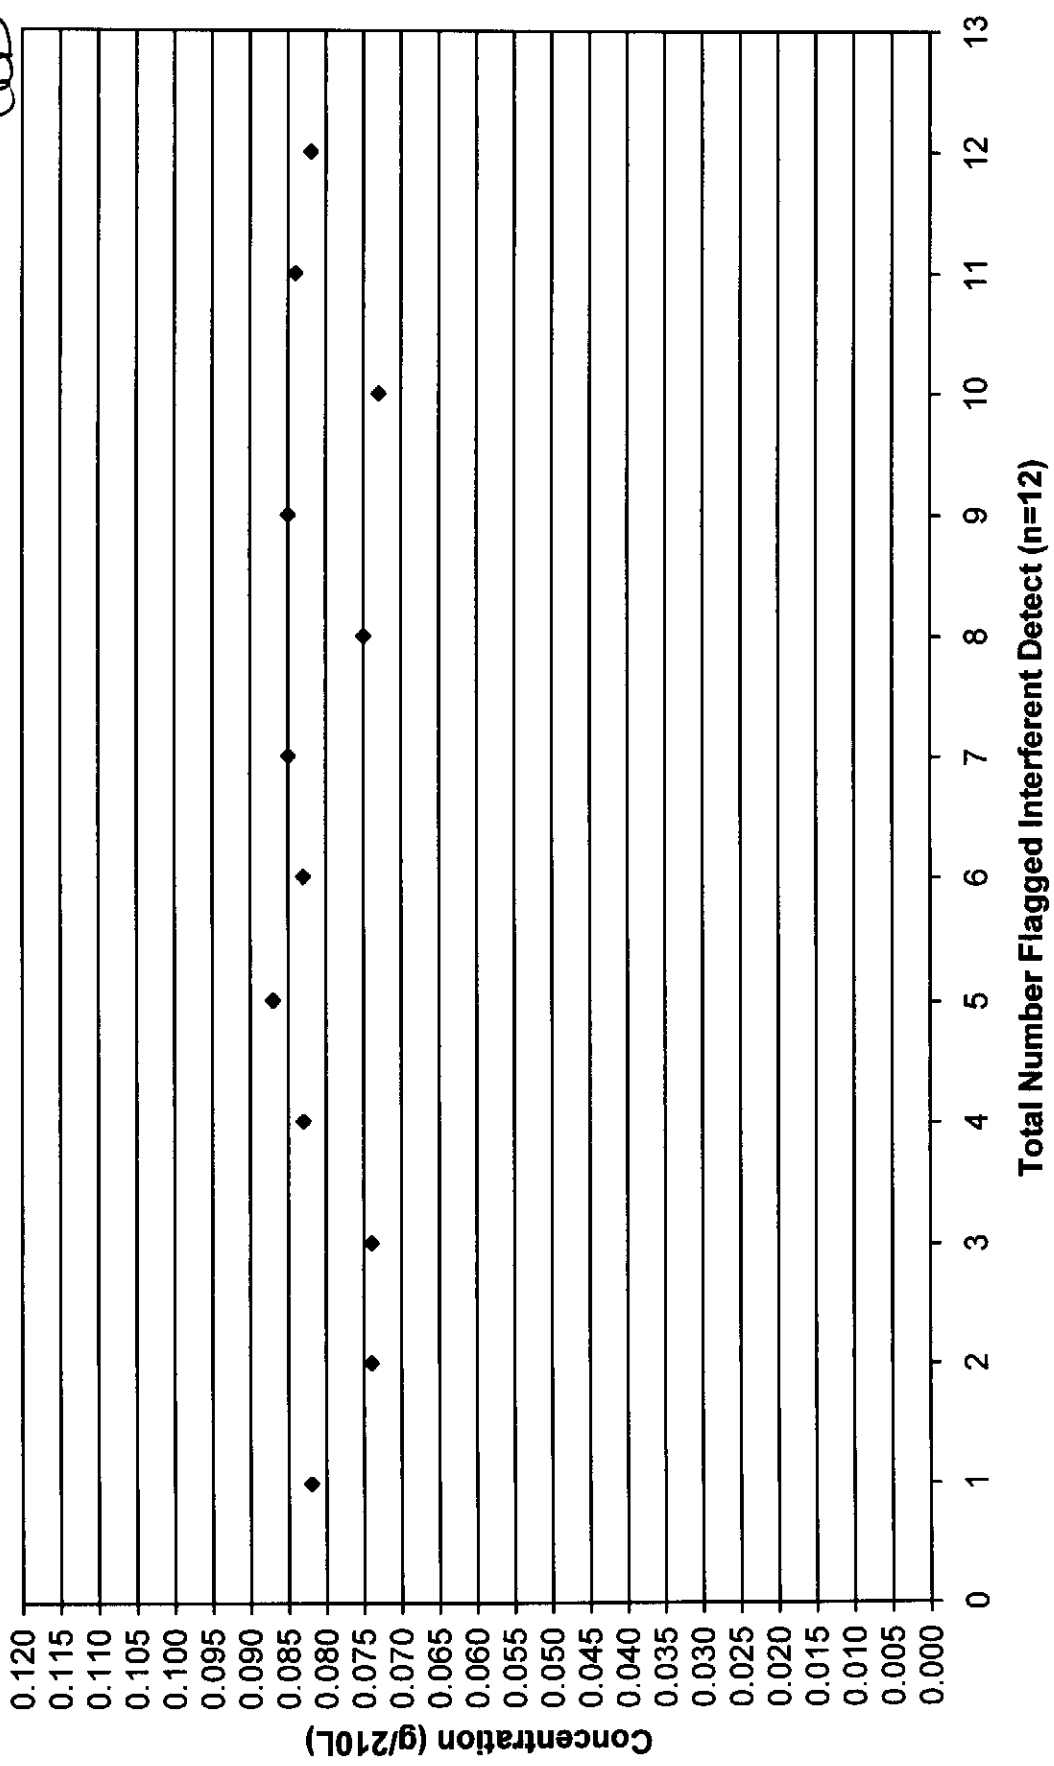

Updated  
11-22-11  
LBB

### February 2011 Updated Control Tests Flagged RFI Detect

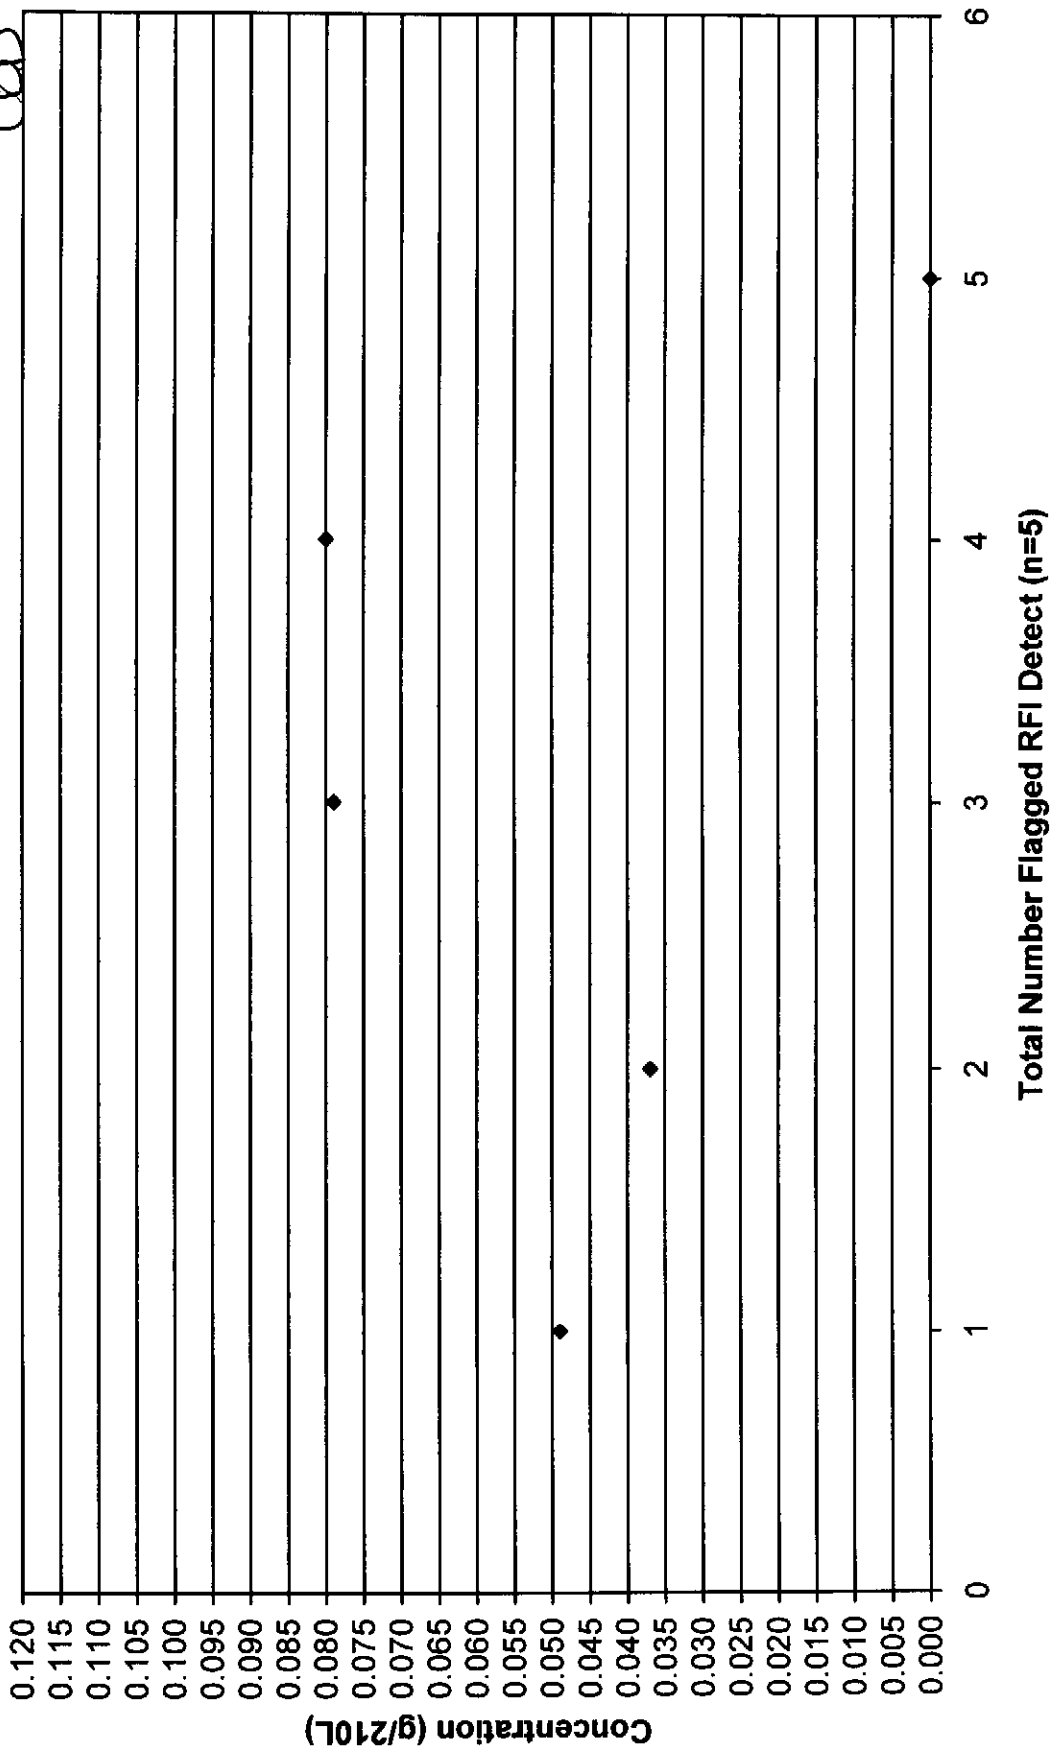

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000872

INSTRUMENT REGISTERED TO: MIAMI PD

SOFTWARE VERSION: 8100.27

BREATH TEST OPERATOR: GARCIA, JUSTIN, B

BREATH TEST OPERATOR AGENCY: Miami PD

ARRESTING OFFICER: MATINEZ, O

ARRESTING OFFICER AGENCY: Miami PD

LAST AGENCY INSPECTION: 02/01/2011

Date or Time Changed: No

DRY GAS STANDARD LOT #: AG002801

DRY GAS EXPIRY DATE: 01/28/2012

VIOLATION CODE: DUI

ARREST TIME: 11:40

GENDER: Male

OBSERVATION PERIOD BEGAN: 12:30

SUBJECT'S LAST NAME: CARNERERO MENENDEZ

DATE/TIME OF TEST: 02/05/2011 12:59:11

---

Diagnostics Check	OK	12:58	
Air Blank	0.000	12:58	
Control Test	0.152	12:59	Control Outside Tolerance
Air Blank		12:59	Improper Sample

---

Data Download Date/Time 03/21/2011 13:40

subject provided  
breath sample during  
control test.  
uob

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000794

INSTRUMENT REGISTERED TO: ST LUCIE COUNTY SO  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: CAGLIONI, DAVID, A  
BREATH TEST OPERATOR AGENCY: St. Lucie County SO  
ARRESTING OFFICER: CAGLIONI, DAVID  
ARRESTING OFFICER AGENCY: St. Lucie County SO  
LAST AGENCY INSPECTION: 01/26/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 685214  
DRY GAS EXPIRY DATE: 10/28/2011  
VIOLATION CODE: DUI  
ARREST TIME: 01:00  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 01:29  
  
DATE/TIME OF TEST: 02/07/2011 01:55:08

SUBJECT'S LAST NAME: CIBERT

Diagnostics Check	OK	01:49	
Air Blank	0.000	01:50	
Control Test	0.083	01:50	
Air Blank	0.000	01:51	
Subject Sample #1	0.127	01:51	
Breath Volume	1.656	01:51	
Air Blank	0.000	01:52	
Air Blank		01:53	RFI Detect
Air Blank	0.000	01:54	
Control Test	0.117	01:54	Control Outside Tolerance
Air Blank		01:55	RFI Detect

Data Download Date/Time 02/19/2011 15:35

*Improper sample  
subject provided  
breath sample  
during control test  
LOB*

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-000794

INSTRUMENT REGISTERED TO: ST LUCIE COUNTY SO  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: CAGLIONI, DAVID, A  
BREATH TEST OPERATOR AGENCY: St. Lucie County SO  
ARRESTING OFFICER: CAGLIONI, DAVID  
ARRESTING OFFICER AGENCY: St. Lucie County SO  
LAST AGENCY INSPECTION: 01/26/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 685214  
DRY GAS EXPIRY DATE: 10/28/2011  
VIOLATION CODE: DUI  
ARREST TIME: 01:00  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 01:29  
DATE/TIME OF TEST: 02/07/2011 02:02:12

SUBJECT'S LAST NAME: CIBERT

---

Diagnostics Check	OK	01:56
Air Blank	0.000	01:56
Control Test	0.082	01:56
Air Blank	0.000	01:57
Subject Sample #1	0.124	01:57
Breath Volume	1.140	01:57
Air Blank	0.000	01:58
Air Blank	0.000	02:00
Subject Sample #2	0.123	02:00
Breath Volume	1.441	02:00
Air Blank	0.000	02:01
Control Test	0.082	02:01
Air Blank	0.000	02:02
Diagnostics Check	OK	02:02

---

Data Download Date/Time 02/19/2011 15:35

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001237

INSTRUMENT REGISTERED TO: POLK COUNTY SO  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: BRADLEY, KEVIN, B  
BREATH TEST OPERATOR AGENCY: Polk County SO  
ARRESTING OFFICER: BRADLEY, KEVIN  
ARRESTING OFFICER AGENCY: Polk County SO  
LAST AGENCY INSPECTION: 02/18/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 770941  
DRY GAS EXPIRY DATE: 05/27/2012  
VIOLATION CODE: DUI  
ARREST TIME: 21:22  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 22:15

SUBJECT'S LAST NAME: VENTUR

DATE/TIME OF TEST: 02/19/2011 23:03:01

Diagnostics Check	OK	22:56	
Air Blank	0.000	22:57	
Control Test	0.083	22:57	
Air Blank	0.000	22:58	
Subject Sample #1	0.126	22:58	
Breath Volume	1.714	22:58	
Air Blank	0.000	22:59	
Air Blank	0.000	23:01	
Subject Sample #2	0.139	23:01	
Breath Volume	2.269	23:01	
Air Blank	0.000	23:02	
Control Test	0.121	23:02	Control Outside Tolerance
Air Blank	0.000	23:03	

Data Download Date/Time 03/30/2011 09:05

subject provided  
breath sample  
during control test  
improper sample  
LAB

**Florida Department of Law Enforcement  
Alcohol Testing Program**

**Subject Test Electronic Data**

CMI, Inc. Intoxilyzer 8000 Serial Number: 80-001237

INSTRUMENT REGISTERED TO: POLK COUNTY SO  
SOFTWARE VERSION: 8100.27  
BREATH TEST OPERATOR: BRADLEY, KEVIN, B  
BREATH TEST OPERATOR AGENCY: Polk County SO  
ARRESTING OFFICER: BRADLEY, KEVIN  
ARRESTING OFFICER AGENCY: Polk County SO  
LAST AGENCY INSPECTION: 02/18/2011

Date or Time Changed: No  
DRY GAS STANDARD LOT #: 770941  
DRY GAS EXPIRY DATE: 05/27/2012  
VIOLATION CODE: DUI  
ARREST TIME: 21:22  
GENDER: Male  
OBSERVATION PERIOD BEGAN: 22:15

SUBJECT'S LAST NAME: VENTUR

DATE/TIME OF TEST: 02/19/2011 23:13:01

---

Diagnostics Check	OK	23:06
Air Blank	0.000	23:07
Control Test	0.082	23:07
Air Blank	0.000	23:08
Subject Sample #1	0.132	23:08
Breath Volume	1.601	23:08
Air Blank	0.000	23:09
Air Blank	0.000	23:11
Subject Sample #2	0.140	23:11
Breath Volume	2.921	23:11
Air Blank	0.000	23:12
Control Test	0.082	23:12
Air Blank	0.000	23:12
Diagnostics Check	OK	23:13

---

Data Download Date/Time 03/30/2011 09:05