

RECEIVED

JUN 26 2017

Florida Department of Law Enforcement Alcohol Testing Program

FDLE
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 09:03

Date of Inspection: 06/23/2017

Serial Number: 80-000949
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000		No
Mouth Alcohol Test: Slope Not Met		No
Interferent Detect Test: Interferent Detect		No
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08g/210L Test (g/210L) Lot#: _____ Exp: _____	0.20g/210L Test (g/210L) Lot#: _____ Exp: _____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: _____ Exp: _____

Number of Simulators Used: _____

Remarks:
SKIPPED AI TO OPERATE INSTRUMENT

SP

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Patrick J Murphy

PATRICK J MURPHY

Signature and Printed Name

06/23/2017
Date

JD

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TALLAHASSEE PD
Time of Inspection: 15:55

Date of Inspection: 04/25/2017

Serial Number: 80-000949
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201507A Exp: 07/14/2017	0.08g/210L Test (g/210L) Lot#: 201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#: 201505A Exp: 05/12/2017	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 34416080A2 Exp: 02/05/2019
0.000	0.047	0.078	0.198	0.080
0.000	0.048	0.078	0.198	0.080
0.000	0.047	0.078	0.199	0.080


Number of Simulators Used: 5

Remarks:

~~RETURN TO EVIDENTIARY SERVICE~~
REMOVED FROM EVIDENTIARY SERVICE FOR DEPARTMENT INSPECTION.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

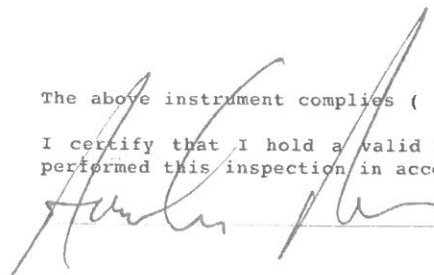

Signature and Printed Name: DAVID A MERESSE

Date: 04/25/2017