

1721
SP

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: PALM BAY P.D.
Time of Inspection: 02:26

Date of Inspection: 04/23/2017

Serial Number: 80-001721
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:26316080A2 Exp: 11/05/2018
0.000	0.047	0.079	0.195	0.081
0.000	0.047	0.079	0.196	0.081
0.000	0.047	0.079	0.197	0.081

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

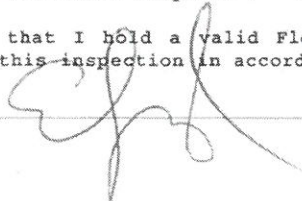

EDWIN J LUTZ
Signature and Printed Name

04/23/2017
Date

1721
48

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED

MAR 28 2017

AGENCY INSPECTION REPORT - INTOXILYZER 8000

FDLE
Alcohol Testing Program

Agency: PALM BAY P.D.
Time of Inspection: 19:29

Date of Inspection: 03/27/2017

Serial Number: 80-001721
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:26316080A2 Exp: 11/05/2018
0.000	0.048	0.078	0.189 / 0.192	0.080
0.000	0.049	0.079	0.191 / 0.192	0.081
0.000	0.049	0.079	0.193 / 0.193	0.081


Number of Simulators Used: 5

Remarks:

20: Control Outside Tolerance. SUSPECT AIR LEAK / SIMULATOR

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

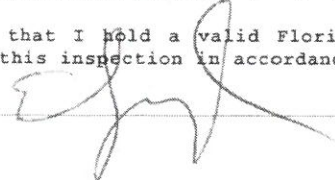

EDWIN J LUTZ
Signature and Printed Name

03/27/2017
Date

SP
1721

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: PALM BAY P.D.
Time of Inspection: 12:19

Date of Inspection: 02/26/2017

Serial Number: 80-001721
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201601F Exp: 01/26/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:24515080A2 Exp: 10/05/2017
0.000	0.049	0.079	0.192	0.079
0.000	0.049	0.079	0.193	0.080
0.000	0.049	0.080	0.193	0.079

Number of Simulators Used: 5

Remarks:

A F / M A : . REPEATED MA

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

EDWIN J LUTZ


Signature and Printed Name

02/26/2017
Date

D. Morgan


PALM BAY P.D.
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-001009
 02/26/2017
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	11:16
Control Test	0.190	11:17
Air Blank	0.000	11:17
Control Test	0.191	11:18
Air Blank	0.000	11:18
Control Test Stats		
Average	0.1905	
Std Dev	0.0007	
Rel Std Dev(%)	0.3712	


 Operator's Signature

PALM BAY P.D.
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-001266
 02/26/2017
 Software: 8100.27


Test	g/210L	Time
Air Blank	0.000	10:47
Control Test	0.047	10:47
Air Blank	0.000	10:48
Control Test	0.047	10:49
Air Blank	0.000	10:49
Control Test Stats		
Average	0.0470	
Std Dev	0.0010	
Rel Std Dev(%)	0.0000	

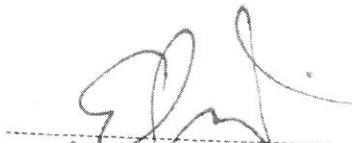
 Operator's Signature

SP1721

PALM BAY P.D.
 Intoxilyzer - Alcohol Analyzer
 Model 8000 SN 80-001721
 02/26/2017
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	10:41
Control Test	0.076	10:42
Air Blank	0.000	10:42
Control Test	0.077	10:43
Air Blank	0.000	10:43
Control Test Stats		
Average	0.0765	
Std Dev	0.0007	
Rel Std Dev(%)	0.9243	


 Operator's Signature