

RECEIVED

Florida Department of Law Enforcement Alcohol Testing Program

DEC 14 2017

FDLE
Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

80-000770
VBA

Agency: Hamilton County SO
Time of Inspection:

Date of Inspection: 10/05/2017

Serial Number: 80-0770
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK			Date and/or Time Adjusted		
Minimum Sample Volume Check: OK			Barometric Pressure Sensor Check: OK		
Alcohol Free Subject Test: 0.000			Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect			Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Standard Deviations				
---------------------	--	--	--	--

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: _____ Number of Simulators Used: _____

Remarks: Instrument could not be inspected due to inability to power on. Sent to repair.

The above instrument complies () does not comply (x) with Chapter 11D-8, FAC.
I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

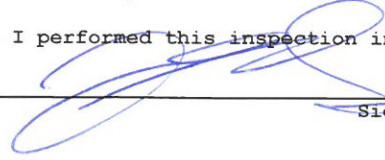
Signature and Printed Name
Date: 10/5/17

ADS
10/11/17
de

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: Hamilton County SO.
 Time of Inspection: 11:55

Date of Inspection: 10/5/17

Serial Number: 80-000770
 Software: 8100.27 *face*

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK			Date and/or Time Adjusted		
Minimum Sample Volume Check: OK			Barometric Pressure Sensor Check: OK		
Alcohol Free Subject Test: 0.000			Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect			Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Standard Deviations				
---------------------	--	--	--	--

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: _____ Number of Simulators Used: _____

Remarks:
Instrument will not power on. Unable to perform D.I.
Being sent to Enforcement Electronics 10/5/17

The above instrument complies () does not comply () with Chapter 11D-8, FAC.
 I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

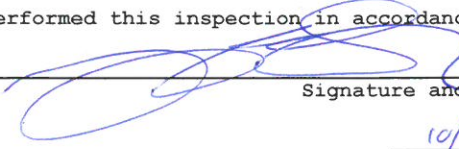

 Signature and Printed Name
10/5/17
 Date
Julie Sharahan

Florida Department of Law Enforcement Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: Hamilton County SO
Time of Inspection:

Serial Number: 80-0770
Software: 8100.27

Date of Inspection: 10/05/2017

✓ BLS

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK			Date and/or Time Adjusted		
Minimum Sample Volume Check: OK			Barometric Pressure Sensor Check: OK		
Alcohol Free Subject Test: 0.000			Mouth Alcohol Test: Slope Not Met		
Interferent Detect Test: Interferent Detect			Diagnostic Check (Post-Inspection): OK		


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: Exp:	0.08g/210L Test (g/210L) Lot#: Exp:	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:

Standard Deviations				
---------------------	--	--	--	--

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: _____ Number of Simulators Used: _____

Remarks: Instrument could not be inspected due to inability to power on. Sent to repair.

The above instrument complies () does not comply (x) with Chapter 11D-8, FAC.
I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

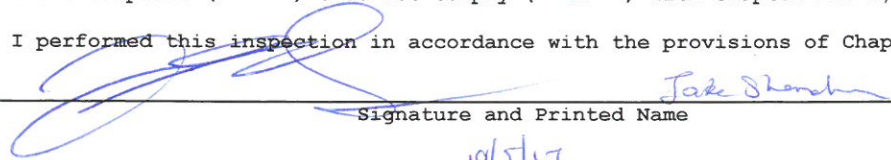

 Signature and Printed Name
 10/5/17

 Date