

Florida Department of Law Enforcement Alcohol Testing Program

SEP 19 2017

FDLE
Alcohol Testing Program

DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.
Time of Inspection: 12:01

Date of Inspection: 09/19/2017

Serial Number: 80-001420
Software: 8100.27

✓BLC

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201707D Exp: 07/25/2019	0.08g/210L Test (g/210L) Lot#:201707E Exp: 07/25/2019	0.20g/210L Test (g/210L) Lot#:201707C Exp: 07/24/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG619605 Exp: 07/14/2018
0.000	0.049	0.080	0.198	0.000 / 0.080
0.000	0.049	0.080	0.198	0.000 / 0.080
0.000	0.049	0.081	0.198	0.000 / 0.080
0.000	0.049	0.081	0.199	0.000 / 0.080
0.000	0.049	0.081	0.198	0.000 / 0.080
0.000	0.049	0.081	0.197	0.000 / 0.080
0.000	0.050	0.081	0.197	0.000 / 0.079
0.000	0.049	0.081	0.198	0.000 / 0.080
0.000	0.050	0.081	0.199	0.000 / 0.079
0.000	0.049	0.081	0.198	0.080 / 0.079
Standard Deviations	0.0004	0.0004	0.0006	0.0252 / 0.0004


Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0004 Number of Simulators Used: 5

Remarks:
08: Control Outside Tolerance DGS NOT CONNECTED RETEST.

PJM

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

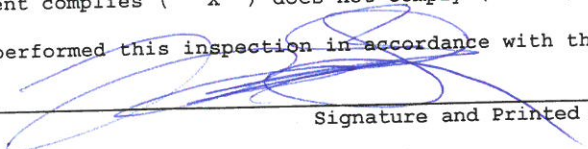

JAKE L SHANAHAN

Signature and Printed Name

09/19/2017
Date

*9/19/17
JD*