

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 14:41

Date of Inspection: 10/08/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.049	0.077	0.195	0.081
0.000	0.049	0.077	0.197	0.081
0.000	0.049	0.078	0.198	0.081

Number of Simulators Used: 5

Remarks:
NA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

10/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 15:29

Date of Inspection: 09/09/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.048	0.078	0.200	0.081
0.000	0.048	0.078	0.200	0.081
0.000	0.049	0.078	0.200	0.081

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



JOANNA N BOWMAN

Signature and Printed Name

09/09/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 11:50

Date of Inspection: 08/03/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.198	0.080
0.000	0.047	0.077	0.199	0.080
0.000	0.047	0.077	0.200	0.080

Number of Simulators Used: 5

Remarks:
N/A

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

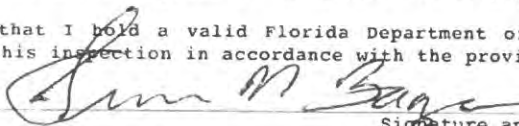

SUSAN M BARGE

Signature and Printed Name

08/03/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED
JUL 18 2018

FDLE
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 17:52

Date of Inspection: 07/06/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.048	0.000 / 0.077	0.198	0.080
0.000	0.048	0.000 / 0.078	0.199	0.081
0.000	0.049	0.000 / 0.078	0.199	0.080

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance SIM WASN'T HOOKED UP TO INLET.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M. Barge

SUSAN M BARGE

Signature and Printed Name

07/06/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

RECEIVED
JUL 18 2018
FDLE
Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP
Time of Inspection: 20:05

Date of Inspection: 05/08/2018

Serial Number: 80-000781
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) <i>201709A</i> Lot#:201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.081
0.000	0.047	0.077	0.199	0.082
0.000	0.048	0.077	0.199	0.081

Number of Simulators Used: 5

Remarks:

A F / M A: TOO MUCH MA

JMB

0.08
210/L
test

Lot# 201709A
JMB

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M Barge

SUSAN M BARGE

Signature and Printed Name

05/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP
Time of Inspection: 20:05

Date of Inspection: 05/08/2018

Serial Number: 80-000781
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) <i>201709A</i> Lot#:201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.081
0.000	0.047	0.077	0.199	0.082
0.000	0.048	0.077	0.199	0.081

Number of Simulators Used: 5

Remarks:

A F / M A: TOO MUCH MA

JMB

 .08
 210/L
 test
 Lot# 201709A
JMB

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M Barge

SUSAN M BARGE

Signature and Printed Name

05/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 20:05

Date of Inspection: 05/08/2018

Serial Number: 80-000781

Software: 8100.27


Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201708A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.199	0.081
0.000	0.047	0.077	0.199	0.082
0.000	0.048	0.077	0.199	0.081

Number of Simulators Used: 5


Remarks:

A F / M A: TOO MUCH MA



The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

05/08/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 19:15

Date of Inspection: 04/05/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:770784 Exp: 04/27/2020
0.000	0.047	0.077	0.197	0.081
0.000	0.048	0.077	0.198	0.081
0.000	0.048	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:
NONE NOTED

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

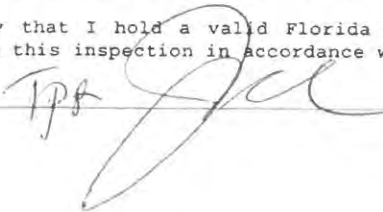

JACOB A MOORE

Signature and Printed Name

04/05/2018
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FHP

Time of Inspection: 02:16

Date of Inspection: 03/20/2018

Serial Number: 80-000781

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 07/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 770784 Exp: 04/27/2020
0.000	0.048	0.078	0.197	0.000 / 0.081
0.000	0.049	0.077	0.199	0.000 / 0.081
0.000	0.048	0.077	0.198	0.081 / 0.081

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance NOT PLUGGED IN.

jm3

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan M Barge

SUSAN M BARGE

Signature and Printed Name

03/20/2018

Date