

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 02:53

Date of Inspection: 12/01/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.049	0.078	0.196	0.081
0.000	0.048	0.078	0.197	0.081
0.000	0.049	0.078	0.196	0.081

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

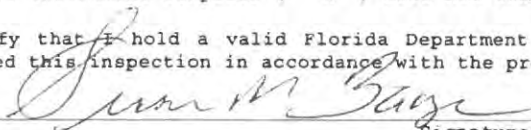

SUSAN M BARGE

Signature and Printed Name

12/01/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:09

Date of Inspection: 11/05/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M. BARGE

Signature and Printed Name

11/05/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 18:54

Date of Inspection: 10/08/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.046	0.076	0.194	0.081
0.000	0.047	0.075	0.196	0.080
0.000	0.047	0.076	0.197	0.081

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

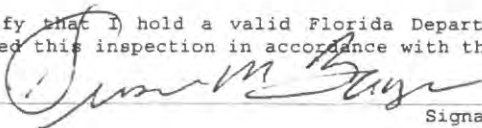

SUSAN M BARGE

Signature and Printed Name

10/08/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:09

Date of Inspection: 11/05/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.078	0.196	0.080
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M. BARGE

Signature and Printed Name

11/05/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:56

Date of Inspection: 09/10/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.048	0.077	0.194	0.080
0.000	0.048	0.078	0.196	0.080
0.000	0.048	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

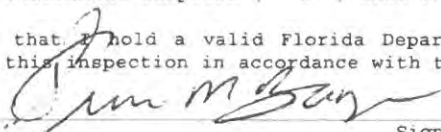

SUSAN M BARGE

Signature and Printed Name

09/10/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 11:14

Date of Inspection: 08/03/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.048	0.077	0.197	0.080
0.000	0.048	0.078	0.197	0.080
0.000	0.048	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:  
N/A

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

08/03/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

**RECEIVED**  
JUL 18 2018  
FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 17:36

Date of Inspection: 07/06/2018

Serial Number: 80-01118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:344160801 Exp: 03/05/20
0.000	0.049	0.078	0.198	0.080
0.000	0.049	0.078	0.200	0.080
0.000	0.049	0.078	0.199	0.080

*2021 km*

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*Susan M Barge*

SUSAN M BARGE

Signature and Printed Name

07/06/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:35

Date of Inspection: 06/14/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 34416080A2 Exp: 02/05/2019
0.000	0.048	0.077	0.198	0.081
0.000	0.048	0.077	0.198	0.081
0.000	0.048	0.077	0.199	0.081

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



Signature and Printed Name

SUSAN M BARGE

06/14/2018  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:52

Date of Inspection: 05/08/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK	Yes	No
Alcohol Free Subject Test 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 01118 Exp: 01/11/18	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201701B Exp: 02/21/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 01118 Exp: 01/11/18
0.000	0.049	0.077	0.194	0.080
0.000	0.049	0.077	0.197	0.080
0.000	0.050	0.077	0.196	0.080

Number of Simulators Used:

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Susan H. [Signature]

Signature and Printed Name

SUSAN H. [Printed Name]

05/08/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:23

Date of Inspection: 04/05/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.049	0.077	0.198	0.080
0.000	0.048	0.077	0.199	0.080
0.000	0.050	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:  
NONE NOTED

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

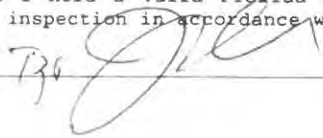

JACOB A MOORE

Signature and Printed Name

04/05/2018  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 19:27

Date of Inspection: 02/02/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#: 201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#: 201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 34416080A2 Exp: 02/05/2019
0.000	0.049	0.079	0.197	0.080
0.000	0.049	0.079	0.197	0.080
0.000	0.050	0.079	0.196	0.080

Number of Simulators Used: 5

Remarks:  
TOO MUCH MA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



SUSAN M BARGE

Signature and Printed Name

02/02/2018  
Date

RECEIVED

# Florida Department of Law Enforcement Alcohol Testing Program

JAN 17 2018

FDLE  
Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: FL HIGHWAY PATROL  
Time of Inspection: 13:24

Date of Inspection: 01/15/2018

Serial Number: 80-001118  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201603D Exp: 03/08/2018	0.08g/210L Test (g/210L) Lot#:201611B Exp: 11/15/2018	0.20g/210L Test (g/210L) Lot#:201604C Exp: 04/05/2018	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:34416080A2 Exp: 02/05/2019
0.000	0.048	0.079	0.197	0.081
0.000	0.048	0.079	0.197	0.082
0.000	0.049	0.079	0.198	0.082

Number of Simulators Used: 5

Remarks:  
NA

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
Signature and Printed Name

SUSAN M BARGE

01/15/2018  
Date