

1207
SP

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HENDRY COUNTY S.O.
Time of Inspection: 21:55

Date of Inspection: 08/22/2018


Serial Number: 80-001207
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:83551 Exp: 10/02/2018
0.000	0.050	0.079	0.198	0.080
0.000	0.050	0.080	0.199	0.080
0.000	0.050	0.080	0.200	0.080

Number of Simulators Used: 5


Remarks:

A F / M A: DID NOT USE ENOUGH MOUTH ALCOHOL. 

RECEIVED
AUG 22 2018
FDLE
Alcohol Testing Program

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


CHRISTOPHER J NORWOOD
Signature and Printed Name

08/22/2018
Date

1207 SP

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HENDRY COUNTY S.O.
Time of Inspection: 23:53

Date of Inspection: 04/18/2018

Serial Number: 80-001207
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:83551 Exp: 10/02/2018
0.000	0.047	0.074 / 0.082	0.198	0.082
0.000	0.048	0.075 / 0.081	0.200	0.082
0.000	0.048	0.076 / 0.080	0.202	0.081


Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance. - small tear in simulator hose. Replaced hose no further issues. (w)

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

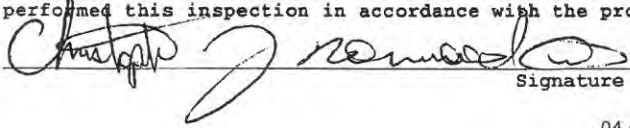

CHRISTOPHER J NORWOOD

Signature and Printed Name

04/18/2018
Date