

Florida Department of Law Enforcement Alcohol Testing Program

Amended
by
Jayson Levy

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: LEVY COUNTY SO
Time of Inspection: 17:07

Date of Inspection: 09/17/2018

Serial Number: 80-001265
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201702B Exp: 02/23/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: AG805701 Exp: 02/26/2020
/ 0.000	0.048	0.079	0.191	0.079
/ 0.000	0.046	0.077	0.196	0.080
/ 0.000	0.045	0.078	0.197	0.079

Number of Simulators Used: 5


Remarks:

00: Ambient Fail.

Ambient Fail - unknown/no fan in use in the
Breath Test Area
J. Levy

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

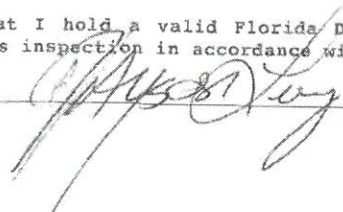

JAYSON I LEVY

Signature and Printed Name

09/17/2018
Date