

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.
Time of Inspection: 09:51

Date of Inspection: 10/09/2018

Serial Number: 80-001418
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201703A Exp: 03/07/2019	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:13917080A3 Exp: 07/05/2019
0.000	0.050	0.080	0.199	0.000 / 0.082
0.000	0.050	0.080	0.200	0.000 / 0.081
0.000	0.050	0.080	0.200	0.000 / 0.081


Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance CHANGED DGS CYL AND REPEATED ^{DGS} Dry Gas standard on second set of testing was 13917080A3, with an expiration date of 07/05/2019 dm

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

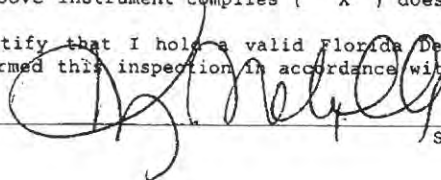

KELLY M MELVILLE

Signature and Printed Name

10/09/2018
Date