



INSTRUMENT PROCESSING SHEET

Agency Orange County SO

S/N 80-001256

Florida Department of Law Enforcement

Date In 9/27/18

DI Completion Date 10/16/18

Ship  P/U  H/D  CMI  EE

<b>Intake</b> Performed By <u>SQC</u> <input checked="" type="checkbox"/> Annual <input type="checkbox"/> Registration <input type="checkbox"/> Return from CMI / EE Visual Inspection: <input checked="" type="checkbox"/> Case <input checked="" type="checkbox"/> Handle <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Dry Gas Shelf <input checked="" type="checkbox"/> Feet <input checked="" type="checkbox"/> Breath Tube <input checked="" type="checkbox"/> Ports <input checked="" type="checkbox"/> Screws Tight Other Equipment/ Accessories: <input type="checkbox"/> Power cord <input type="checkbox"/> Printer Cable <input checked="" type="checkbox"/> Static Bag <input type="checkbox"/> 12V DC Cable Notes: _____	<b>Quality Checks</b> Performed By <u>[Signature]</u> <input checked="" type="checkbox"/> Breath Tube Screen <input checked="" type="checkbox"/> Replace External O-Rings <input checked="" type="checkbox"/> Instrument Set Up Verified <input checked="" type="checkbox"/> R-Value <u>202</u> <input checked="" type="checkbox"/> Flow Verification (L/s) Flow Column # <u>ATP102</u> 32 mm <u>152</u> (.139 - .169) 36 mm <u>167</u> (.156 - .190) 53 mm <u>238</u> (.228 - .278) 103 mm <u>507</u> (.447 - .547) <input checked="" type="checkbox"/> Barometric Pressure Check Gauge ID # <u>25427</u> <input checked="" type="checkbox"/> Stability Checks	<b>Flow Calibration</b> Performed By _____ Flow Column # _____ <input type="checkbox"/> 5L/min - 17mm <input type="checkbox"/> 15L/min - 53mm <input type="checkbox"/> 30L/min - 103mm <input type="checkbox"/> R-Value _____ <input type="checkbox"/> Post Calibration Verification (L/s) Flow Column # _____ 32 mm _____ (.139 - .169) 36 mm _____ (.156 - .190) 53 mm _____ (.228 - .278) 103 mm _____ (.447 - .547)
---	--	--

**Final Release Date**

**FDLE**

**OCT 16 2018**

**Alcohol Testing Program**

Simulator	Serial #	Lot #/Exp
0.050	SD1021	201707D 7/25/19
0.080	DR1275	201707E 7/25/19
0.200	SD1013	201707C 7/24/19
0.080 DGS	N/A	AG805701 2/26/20

**Maintenance** Performed By \_\_\_\_\_

Battery Replacement  
 Dry Gas Regulator Replacement  
 Breath Tube Replacement  
 Other \_\_\_\_\_

**Temperature Checks** Performed By [Signature]

Lab Temp °C 21.2  
 External Digital Therm. ID#: 300503  
 34°C +/- .2 Serial #: SD1021  
 34°C +/- .2 Serial #: DR1275  
 34°C +/- .2 Serial #: SD1013

**Calibration Adjustment** Performed By [Signature]

Barometric Pressure Gauge 1017 ID # 25427

Simulator	Serial Number	Lot Number	Expiration
0.000	G2880	N/A	N/A
0.040	SD1022	17410	12/6/19
0.100	SD3964	18070	2/26/20
0.200	SD1025	17340	10/9/19
0.300	SD1024	18110	4/2/20
0.080 DGS	N/A	17817080A2	8/5/19

**Department Inspection** Performed By [Signature]

Barometric Pressure ID# 25427-28662  
 Gauge 1017 Instrument 1017 K18  
 Mouth Alcohol Solution Lot # 2016-C  
 Acetone Stock Solution Lot # 2018-A

Simulator	Serial Number
0.000	G-11621
Interferent	DR3855
0.050	SD1021
0.080	DR1275
0.200	SD1013

Post Calibration Adjustment Stability Checks

Simulator	Serial Number	Lot Number	Expiration
0.050	SD1021	201707D	7/25/19
0.080	DR1275	201707E	7/25/19
0.200	SD1013	201707C	7/24/19
0.080 DGS	N/A	AG805701	2/26/20

**Attachments**

Form 41  Post-Stability Checks  
 Stability Checks  Flow Calibration  
 Calibration Certificate  Form 40  
 Calibration Adjustment  Other \_\_\_\_\_

Notes/Suggested Service: \_\_\_\_\_

\_\_\_\_\_


\_\_\_\_\_

\_\_\_\_\_

\_\_\_\_\_

Instrument Complies with Chapter 11D-8, FAC  
 Instrument Does Not Comply with Chapter 11D-8, FAC  
 Return to/Place into Evidentiary Use  
 Remain Out of Evidentiary Use  
 Conduct an Agency Inspection Before Evidentiary Use

[Signature] 10/16/18 Tech Review / Date  
[Signature] 10/14/18 Admin Review / Date

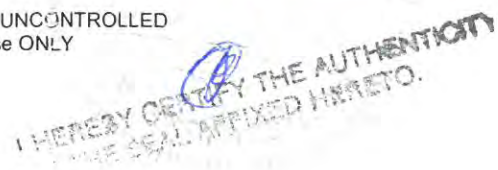

# Florida Department of Law Enforcement Alcohol Testing Program

## DEPARTMENT INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.  
Time of Inspection: 10:37

Date of Inspection: 10/16/2018

Serial Number: 80-001256  
Software: 8100.27

Check or Test	YES	NO	Check or Test	YES	NO
Diagnostic Check (Pre-Inspection): OK	Yes		Date and/or Time Adjusted		No
Minimum Sample Volume Check: OK	Yes		Barometric Pressure Sensor Check: OK	Yes	
Alcohol Free Subject Test: 0.000	Yes		Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes		Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201707D Exp: 07/25/2019	0.08g/210L Test (g/210L) Lot#:201707E Exp: 07/25/2019	0.20g/210L Test (g/210L) Lot#:201707C Exp: 07/24/2019	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:AG805701 Exp: 02/26/2020
0.000	0.049	0.082	0.201	0.079
0.000	0.049	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.203	0.080
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.202	0.079
0.000	0.050	0.082	0.203	0.079

Standard Deviations	0.0004	0.0000	0.0005	0.0003
---------------------	--------	--------	--------	--------

Average Standard Deviation of 0.05, 0.08 and 0.20 g/210L Tests: 0.0003 Number of Simulators Used: 5

Remarks:

*Boym*

The above instrument complies (  ) does not comply (  ) with Chapter 11D-8, FAC.

I certify that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



JAKE L SHANAHAN

Signature and Printed Name

10/16/2018  
Date

I HEREBY CERTIFY THE AUTHENTICITY OF THE SEAL APPLIED HERETO.

*10/16/18  
JO*

80-001256  
 Stability Checks  
 10/15/18

INTOXILYZER 8000  
 Instrument Initialization  
 06:31 10/15/2018

ORANGE COUNTY S.O.  
 Intoxilyzer - Alconol Analyzer  
 Model 8000  
 10/15/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:11
Control Test	0.046	07:11
Air Blank	0.000	07:12
Control Test	0.046	07:13
Air Blank	0.000	07:13
Control Test	0.046	07:14
Air Blank	0.000	07:14
Control Test Stats		
Average	0.0460	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

*Becker*

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alconol Analyzer  
 Model 8000  
 10/15/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:00
Control Test	0.079	07:00
Air Blank	0.000	07:01
Control Test	0.079	07:01
Air Blank	0.000	07:02
Control Test	0.079	07:02
Air Blank	0.000	07:03
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

*DSS*

Operator's Signature

*RAM 10/16/18*

ORANGE COUNTY S.O.  
 Intoxilyzer - Alconol Analyzer  
 Model 8000  
 10/15/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:25
Control Test	0.200	07:26
Air Blank	0.000	07:26
Control Test	0.200	07:27
Air Blank	0.000	07:27
Control Test	0.200	07:28
Air Blank	0.000	07:28
Control Test Stats		
Average	0.2000	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alconol Analyzer  
 Model 8000  
 10/15/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:19
Control Test	0.046	07:20
Air Blank	0.000	07:20
Control Test	0.047	07:21
Air Blank	0.000	07:21
Control Test	0.046	07:22
Air Blank	0.000	07:22
Control Test Stats		
Average	0.0463	
Std Dev	0.0006	
Rel Std Dev(%)	1.2461	

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alconol Analyzer  
 Model 8000  
 10/15/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	07:30
Control Test	0.078	07:31
Air Blank	0.000	07:31
Control Test	0.078	07:32
Air Blank	0.000	07:32
Control Test	0.079	07:33
Air Blank	0.000	07:34
Control Test Stats		
Average	0.0783	
Std Dev	0.0006	
Rel Std Dev(%)	0.7370	

Operator's Signature

HEREBY CERTIFY THE AUTHENTICITY OF THE SEAL AFFIXED HERETO.



Florida Department of Law Enforcement  
 Alcohol Testing Program  
 2729 Fort Knox Blvd.  
 Bldg. 2, Suite 1300  
 Tallahassee, FL 32308

# Calibration Certificate

This is to certify the calibration of Intoxilyzer 8000 serial number 80-001256, manufactured by CMI, Inc. was calibrated in accordance with FDLE/ATP Form 36 - Department Inspection Procedures - Intoxilyzer 8000.

Serial Number:	<u>80-001256</u>	UNCERTAINTY* $\pm$	
Owning Agency:	<u>ORANGE COUNTY S.O.</u>	0.050 g/ 210 L	0.004
Calibration Date:	<u>10/16/2018</u>	0.080 g/ 210 L	0.005
Calibration Time:	<u>10:37</u>	0.200 g/ 210 L	0.008
		0.080 g/ 210 L Dry Gas Control	0.005

All results are reported in g/ 210 L.  
 Bias is limited by calibration acceptance criteria. All calibration results must be within  $\pm$  0.005 or 5%, whichever is greater, of the target alcohol concentration.  
 \*Uncertainty is based on fleet-wide data and is expressed to a 99.73% level of confidence (k=3).

**TRACEABILITY INFORMATION**  
 This instrument was calibrated using solutions prepared by Alcohol Countermeasure Systems, Inc. (ACS). ACS prepared and certified these CRMs in accordance with ISO 17034 and ISO/ IEC 17025 Standards.

Simulator temperatures are traceable to NIST. Thermometer temperatures are checked with NIST traceable Eutechnics 4400 digital thermometers calibrated by Precision Metrology in accordance with ISO/ IEC 17025 standards.

Dry gas control measurements are traceable to NIST through the uses of CRMs supplied by an accredited CRM supplier. The supplier of dry gas standard controls prepared and certified the CRMs in accordance with ISO Guide 34 and ISO/ IEC 17025 standards.

This document shall not be reproduced except in full, without written approval of the Florida Department of Law Enforcement Alcohol Testing Program.

10/16/2018 Date

**JAKE L SHANAHAN,**  
 Department Inspector

FDLE/ATP Form 69 July 2018  
 Issuing Authority: Alcohol Testing Program

*Service • Integrity • Respect • Quality*

*Ryan*  
*10/16/18*  
 I HEREBY CERTIFY THE AUTHENTICITY OF THE SEAL AFFIXED HERETO.

80-001256  
Cal. Adjust  
10/16/18

INTOXILYZER 8000  
Instrument Initialization  
06:47 10/16/2018

ORANGE COUNTY S.O.  
Intoxilyzer - Alcohol Analyzer  
Model: 8000 SN 80-001256  
10/16/2018 07:28:23

\*\*\*\*\* AUTO CAL DATA \*\*\*\*\*  
<<<<< CHANNEL 1 >>>>>  
Sol Val = 0.0000 mg/l or 0.000 g/210L  
% Abs = 0.074  
Std Dev = 0.01 Rel Std Dev = 17.19  
Sol Val = 0.1905 mg/l or 0.040 g/210L  
% Abs = 0.819  
Std Dev = 0.02 Rel Std Dev = 2.22  
Sol Val = 0.4762 mg/l or 0.100 g/210L  
% Abs = 1.975  
Std Dev = 0.00 Rel Std Dev = 0.24  
Sol Val = 0.9524 mg/l or 0.200 g/210L  
% Abs = 3.738  
Std Dev = 0.01 Rel Std Dev = 0.39  
Sol Val = 1.4286 mg/l or 0.300 g/210L  
% Abs = 5.529  
Std Dev = 0.02 Rel Std Dev = 0.39  
Zero Order Coef = -186.61  
First Order Coef = 2500.04  
Second Order Coef = 21.82  
Standard Deviation = 50.398657

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 6.8420 (-0.0110)  
Sample #2 = 6.8740 (0.0150)  
Sample #3 = 6.8990 (0.0180)  
Sample #4 = 6.9130 (0.0250)  
Avg % Abs = 6.8953 (0.0193)  
STD DEV = 0.0198 (0.0051)  
REL STD DEV = 0.287 (26.543)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sol Value = 0.300 g/210L \*\*\*  
Fit value = 1.4286 mg/l %%%  
Samples Taken = 4, Discarded = 1  
Sum Io = 12596, Sum Io = 13025

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 1.5150 (-0.0150)  
Sample #2 = 1.5310 (0.0050)  
Sample #3 = 1.5380 (0.0030)  
Sample #4 = 1.5400 (0.0010)  
Avg % Abs = 1.5363 (-0.0003)  
STD DEV = 0.0047 (0.0042)  
REL STD DEV = 0.308 (1249.000)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sol Value = 0.100 g/210L \*\*\*  
Fit value = 0.4762 mg/l %%%  
Samples Taken = 4, Discarded = 1  
Sum Io = 12611, Sum Io = 13031

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 1.9860 (-0.0360)  
Sample #2 = 1.9730 (-0.0230)  
Sample #3 = 1.9710 (0.0270)  
Sample #4 = 1.9800 (0.0180)  
Avg % Abs = 1.9747 (0.0073)  
STD DEV = 0.0047 (0.0267)  
REL STD DEV = 0.239 (363.437)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 9.9700 (0.0070)  
Sample #2 = 10.0290 (0.0150)  
Sample #3 = 10.0540 (0.0130)  
Sample #4 = 10.0750 (0.0220)  
Avg % Abs = 10.0527 (0.0167)  
STD DEV = 0.0230 (0.0047)  
REL STD DEV = 0.229 (28.355)

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 3.6450 (-0.0160)  
Sample #2 = 3.6380 (-0.0010)  
Sample #3 = 3.6510 (0.0110)  
Sample #4 = 3.6750 (0.0050)  
Avg % Abs = 3.6547 (0.0050)  
STD DEV = 0.0188 (0.0060)  
REL STD DEV = 0.514 (120.000)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.1250 (-0.0030)  
Sample #2 = 0.1000 (0.0220)  
Sample #3 = 0.1180 (0.0320)  
Sample #4 = 0.1060 (0.0490)  
Avg % Abs = 0.1080 (0.0343)  
STD DEV = 0.0092 (0.0137)  
REL STD DEV = 8.486 (39.758)

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.1020 (-0.0160)  
Sample #2 = 0.0850 (0.0620)  
Sample #3 = 0.0760 (0.0500)  
Sample #4 = 0.0600 (0.1340)  
Avg % Abs = 0.0737 (0.1003)  
STD DEV = 0.0127 (0.0362)  
REL STD DEV = 17.189 (36.106)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 3.7220 (-0.0230)  
Sample #2 = 3.7240 (0.0290)  
Sample #3 = 3.7530 (0.0230)  
Sample #4 = 3.7380 (0.0560)  
Avg % Abs = 3.7383 (0.0360)  
STD DEV = 0.0145 (0.0175)  
REL STD DEV = 0.388 (48.829)

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 8.0160 (0.0030)  
Sample #2 = 0.7980 (0.0410)  
Sample #3 = 0.8260 (0.0680)  
Sample #4 = 0.8320 (0.0620)  
Avg % Abs = 0.8187 (0.0570)  
STD DEV = 0.0181 (0.0142)  
REL STD DEV = 2.217 (24.873)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.040 g/210L \*\*\*  
Fit value = 0.1905 mg/l %%%  
Samples Taken = 4, Discarded = 1  
Sum Io = 12631, Sum Io = 13038

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.8160 (0.0030)  
Sample #2 = 0.7980 (0.0410)  
Sample #3 = 0.8260 (0.0680)  
Sample #4 = 0.8320 (0.0620)  
Avg % Abs = 0.8187 (0.0570)  
STD DEV = 0.0181 (0.0142)  
REL STD DEV = 2.217 (24.873)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 10.0527 (0.0167)  
Sample #2 = 10.0527 (0.0167)  
Sample #3 = 10.0527 (0.0167)  
Sample #4 = 10.0527 (0.0167)  
Avg % Abs = 10.0527 (0.0167)  
STD DEV = 0.0230 (0.0047)  
REL STD DEV = 0.229 (28.355)

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 3.6547 (0.0050)  
Sample #2 = 3.6547 (0.0050)  
Sample #3 = 3.6547 (0.0050)  
Sample #4 = 3.6547 (0.0050)  
Avg % Abs = 3.6547 (0.0050)  
STD DEV = 0.0188 (0.0060)  
REL STD DEV = 0.514 (120.000)

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.040 g/210L \*\*\*  
Fit value = 0.1905 mg/l %%%  
Samples Taken = 4, Discarded = 1  
Sum Io = 12631, Sum Io = 13038

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 0.8160 (0.0030)  
Sample #2 = 0.7980 (0.0410)  
Sample #3 = 0.8260 (0.0680)  
Sample #4 = 0.8320 (0.0620)  
Avg % Abs = 0.8187 (0.0570)  
STD DEV = 0.0181 (0.0142)  
REL STD DEV = 2.217 (24.873)

Solution Stats Quadratic Fit Chan 1  
Act Fit Residual  
g/210L g/210L g/210L  
0.000 -0.000 0.0000  
0.040 0.040 0.0002  
0.100 0.101 -0.0009  
0.200 0.199 0.0009  
0.300 0.300 -0.0003

Sol Value = 0.080 g/210L \*\*\*  
Fit value = 0.3810 mg/l %%%  
Samples Taken = 4, Discarded = 1

\*\*\*\*\* CHANNEL 1  
Sample #1 = 3302.00  
Sample #2 = 3305.00  
Sample #3 = 3387.00  
Sample #4 = 3380.00  
Average Result = 3357.3333  
STD DEV = 45.4569  
REL STD DEV = 1.354

\*\*\*\*\* CHANNEL 2  
Sample #1 = 3403.00  
Sample #2 = 3426.00  
Sample #3 = 3446.00  
Sample #4 = 3441.00  
Average Result = 3437.6667  
STD DEV = 10.4083  
REL STD DEV = 0.303

\*\*\*\*\*  
Dry Gas H2O Adjust Results \*\*\*\*\*  
Barometric Pressure = 1017  
3 um H2O Adjust (mg/l\*10,000) = 452  
9 um H2O Adjust (mg/l\*10,000) = 372  
\*\*\*\*\* AUTO CAL PASS

Solution Stats Quadratic Fit Chan 1  
Act Fit Residual  
g/210L g/210L g/210L  
0.000 -0.000 0.0000  
0.040 0.039 0.0005  
0.100 0.102 -0.0015  
0.200 0.199 0.0012  
0.300 0.300 -0.0004

Sol Value = 0.300 g/210L \*\*\*  
Fit value = 1.4286 mg/l %%%  
Samples Taken = 4, Discarded = 1  
Sum Io = 12596, Sum Io = 13025

\*\*\*\*\* CHANNEL 1 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 5.4620 (0.0040)  
Sample #2 = 5.5080 (0.0330)  
Sample #3 = 5.5290 (0.0200)  
Sample #4 = 5.5510 (0.0300)  
Avg % Abs = 5.5293 (0.0277)  
STD DEV = 0.0215 (0.0068)  
REL STD DEV = 0.389 (24.603)

\*\*\*\*\* CHANNEL 2 >>>>>  
Sample % Abs (% Abs Ref)  
Sample #1 = 9.9700 (0.0070)  
Sample #2 = 10.0290 (0.0150)  
Sample #3 = 10.0540 (0.0130)  
Sample #4 = 10.0750 (0.0220)  
Avg % Abs = 10.0527 (0.0167)  
STD DEV = 0.0230 (0.0047)  
REL STD DEV = 0.229 (28.355)

10/16/18  
BY CERTIFY THE AUTHORITY  
OF THE SEAL APPLIED HERETO.

80-001256  
 Cal adjust Post  
 Stability Checks  
 10/16/18

ORANGE COUNTY S.O.  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-001256  
 10/16/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:17
Control Test	0.079	08:17
Air Blank	0.000	08:17
Control Test	0.079	08:18
Air Blank	0.000	08:18
Control Test	0.079	08:18
Air Blank	0.000	08:19
Control Test Stats		
Average	0.0790	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

*DS*

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-001256  
 10/16/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:26
Control Test	0.049	08:27
Air Blank	0.000	08:28
Control Test	0.049	08:28
Air Blank	0.000	08:29
Control Test	0.049	08:29
Air Blank	0.000	08:29
Control Test	0.049	08:30
Control Test Stats		
Average	0.0490	
Std Dev	0.0000	
Rel Std Dev(%)	0.0000	

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-001256  
 10/16/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:34
Control Test	0.081	08:35
Air Blank	0.000	08:35
Control Test	0.081	08:36
Air Blank	0.000	08:36
Control Test	0.082	08:37
Air Blank	0.000	08:38
Control Test Stats		
Average	0.0813	
Std Dev	0.0006	
Rel Std Dev(%)	0.7099	

Operator's Signature

ORANGE COUNTY S.O.  
 Intoxilyzer - Alcohol Analyzer  
 Model 8000 SN 80-001256  
 10/16/2018  
 Software: 8100.27

Test	g/210L	Time
Air Blank	0.000	08:42
Control Test	0.201	08:43
Air Blank	0.000	08:43
Control Test	0.200	08:44
Air Blank	0.000	08:44
Control Test	0.200	08:45
Air Blank	0.000	08:45
Control Test Stats		
Average	0.2003	
Std Dev	0.0006	
Rel Std Dev(%)	0.2882	

Operator's Signature

10/16/18

I HEREBY CERTIFY THE AUTHORITY OF THE SEAL AFFIXED HERETO.