

# Florida Department of Law Enforcement Alcohol Testing Program

80-000968  
B/K

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 14:57

Date of Inspection: 12/30/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.053	0.076	0.196	0.080
0.000	0.052	0.077	0.196	0.080
0.000	0.052	0.077	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

12/30/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

80-000968  
BK

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 13:54

Date of Inspection: 11/26/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.050	0.078	0.199	0.079
0.000	0.051	0.078	0.199	0.079
0.000	0.050	0.079	0.199	0.080

Number of Simulators Used: 4

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*D. Lyons*

DANIEL E LYONS

Signature and Printed Name

11/26/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 22:10

Date of Inspection: 09/10/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.077	0.194	0.079
0.000	0.048	0.077	0.194	0.080
0.000	0.047	0.078	0.195	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS  
Signature and Printed Name

09/10/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 22:10

Date of Inspection: 09/10/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.077	0.194	0.079
0.000	0.048	0.077	0.194	0.080
0.000	0.047	0.078	0.195	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

  
\_\_\_\_\_  
Signature and Printed Name

DANIEL E LYONS

09/10/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 20:38

Date of Inspection: 08/02/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.077	0.194	0.079
0.000	0.047	0.078	0.194	0.080
0.000	0.047	0.077	0.195	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

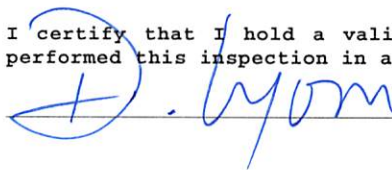

DANIEL E LYONS

Signature and Printed Name

08/02/2019  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

7/3/19  
JH

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 01:33

Date of Inspection: 07/02/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.046	0.077	0.196	0.080
0.000	0.047	0.078	0.198	0.080
0.000	0.047	0.078	0.199	0.080

Number of Simulators Used: 5

**Remarks:**

AF/MA: Range Exceeded. ERROR FOR M/A TEST. RINSED, RETESTED.

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyons

DANIEL E LYONS

Signature and Printed Name

07/02/2019

Date

## Graham, Thomas

---

**From:** Dan Lyons <dlyo@OSCEOLA.ORG>  
**Sent:** Tuesday, July 02, 2019 10:47 PM  
**To:** Graham, Thomas; 'Atkinson, Karsona'; 'McKnight, Jamie (JMcknight@sao9.org)'; 'SherryForcier@flhsmv.gov'  
**Subject:** Monthly Intox Inspections, July 2019  
**Attachments:** 02 July 2019 Monthly Intox Inspec.pdf  
  
**Follow Up Flag:** FollowUp  
**Flag Status:** Completed

ALCON,

Agency Inspection Report completed 07/02/2019 on the following instruments;  
80-000966, 80-000968, 80-001715, 80-003935, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-000966, 0.08g/210L Test, received an Outside Tolerance, I began the test without connecting the Simulator. I connected the simulator and continued the test. The instrument was re-tested. In reference to 0.20g/210L Test, Received an Outside Tolerance, I re-set the Simulators lines and lid and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-000968 the AF/MA test, received a Range Exceeded. I rinsed with the mouth alcohol solution and provided that sample right after rinsing. It showed Range Exceeded. I allowed time, rinsed and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

All intox inspections are complete and in compliance with 11D-8.

V/R

Dan Lyons  
Osceola County Sheriff's Office  
Spec Ops/Traffic/DUI Enforcement Unit  
Agency 407-348-1100  
Agency Cell 407-269-1980  
Cell 321-960-2066

---

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

# Florida Department of Law Enforcement Alcohol Testing Program

6/13/19  
JO

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 21:32

Date of Inspection: 06/11/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.046	0.075	0.192	0.079
0.000	0.046	0.076	0.193	0.078
0.000	0.047	0.076	0.193	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

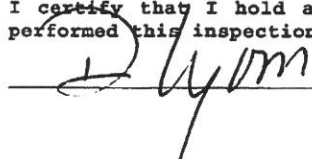

DANIEL E LYONS

Signature and Printed Name

06/11/2019  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

5/17/19  
JL

Agency: OSCEOLA CORRECTIONS  
Time of Inspection: 13:53

Date of Inspection: 05/15/2019

Serial Number: 80-000968  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.076	0.194	0.080
0.000	0.048	0.076	0.195	0.081
0.000	0.048	0.076	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyon

DANIEL E LYONS

Signature and Printed Name

05/15/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

5/3/19  
JO

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 04:42

Date of Inspection: 05/02/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.075	0.192	0.079
0.000	0.048	0.076	0.196	0.079
0.000	0.048	0.076	0.196	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( X ) does not comply ( ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*D. Lyons*

DANIEL E LYONS

Signature and Printed Name

05/02/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

4/8/19  
JO

Agency: OSCEOLA CORRECTIONS  
Time of Inspection: 18:29

Date of Inspection: 04/03/2019

Serial Number: 80-000968  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.049	0.077	0.197	0.080
0.000	0.049	0.078	0.197	0.080
0.000	0.049	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

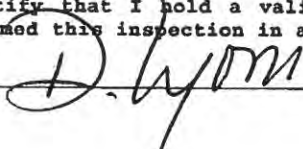

DANIEL E LYONS

Signature and Printed Name

04/03/2019  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

3/19/19  
JL

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS  
Time of Inspection: 23:43

Date of Inspection: 03/18/2019

Serial Number: 80-000968  
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.078	0.198	0.079
0.000	0.049	0.078	0.199	0.079
0.000	0.048	0.078	0.199	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*D Lyons*

DANIEL E LYONS

Signature and Printed Name

03/18/2019  
Date



# Florida Department of Law Enforcement Alcohol Testing Program

2/15/19  
JO

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 19:24

Date of Inspection: 02/07/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.046	0.076	0.191	0.079
0.000	0.046	0.075	0.192	0.080
0.000	0.046	0.075	0.192	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

*D Lyons*

DANIEL E LYONS  
Signature and Printed Name

02/07/2019  
Date

# Florida Department of Law Enforcement Alcohol Testing Program

1/25/19  
JD

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 23:29

Date of Inspection: 01/24/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.047	0.076	0.192	0.079
0.000	0.048	0.076	0.193	0.079
0.000	0.048	0.076	0.193	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

01/24/2019

Date

# Florida Department of Law Enforcement Alcohol Testing Program

1/7/19  
JO

## AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS

Time of Inspection: 22:19

Date of Inspection: 01/06/2019

Serial Number: 80-000968

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.077	0.196	0.079
0.000	0.048	0.078	0.196	0.080
0.000	0.048	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:

AF/MA;RISD MOUTH ALCOHOL SNM READING, RETESTED

The above instrument complies ( ☒ ) does not comply ( ☐ ) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyons

DANIEL E LYONS

01/06/2019  
Date