

Florida Department of Law Enforcement Alcohol Testing Program

6/12/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 14:51

Date of Inspection: 06/11/2019

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#: 201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 32518080A2 Exp: 02/05/2021
0.000	0.047	0.077	0.196	0.079
0.000	0.047	0.078	0.198	0.080
0.000	0.048	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:
Time-Date changed. BACK IN SERVICE AFTER ANNUAL INSPECTION

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

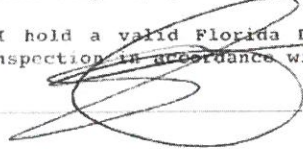

STEVE GASSEN

Signature and Printed Name

06/11/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

5/2/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 15:24

Date of Inspection: 04/30/2019

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#: 201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 32518080A2 Exp: 02/05/2021
0.000	0.048	0.077	0.197	0.079
0.000	0.048	0.078	0.198	0.079
0.000	0.049	0.079	0.199	0.080

Number of Simulators Used: 5

Remarks:
CLEANED AREA

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

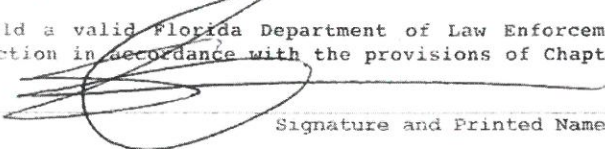

 Signature and Printed Name

STEVE GASSEN

04/30/2019
Date

Graham, Thomas

From: Alcohol Testing Program
Sent: Wednesday, May 01, 2019 7:38 AM
To: Graham, Thomas
Subject: FW: April 2019 AI
Attachments: April 2019 Inspection.pdf



80-001065
5/2/19
JA

Follow Up Flag: FollowUp
Flag Status: Flagged

From: Steve Gassen [mailto:sgassen@tspd.us]
Sent: Tuesday, April 30, 2019 3:39 PM
To: Alcohol Testing Program
Subject: April 2019 AI

Just an FYI I tried to upload the AI and it never answered.


STEVE GASSEN
POLICE OFFICER



TARPON SPRINGS
POLICE DEPARTMENT

"Building a Better Future through Excellence in Policing"

444 South Huey Avenue
Tarpon Springs, FL 34689
(727) 938-2849 – Main
(727) 939-4534 - Direct
(727) 937-0193 – Fax
sgassen@tspd.us



Please Note: The State of Florida has a very broad public records law under chapter 119. Most written material to or from City officials regarding City business are public records and available to the public or media upon request. Your e-mail communications and/or e-mail attachments may be subject to public disclosure.

Florida Department of Law Enforcement Alcohol Testing Program

2/27/19
JE

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 21:55

Date of Inspection: 02/26/2019

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#: 201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 32518080A2 Exp: 02/05/2021
0.000	0.048	0.077	0.197	0.080
0.000	0.048	0.077	0.198	0.080
0.000	0.048	0.079	0.198	0.080


Number of Simulators Used: 5

Remarks:

Inl Det: Ambient Fail ACETONE IN THE AREA.

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

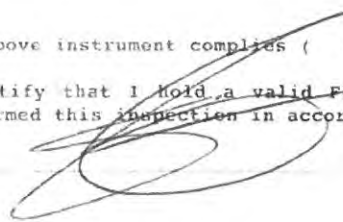

Signature and Printed Name STEVE P GASSEN

Date 02/26/2019