

1207
SP

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HENDRY COUNTY S.O.
Time of Inspection: 02:15

Date of Inspection: 07/12/2019

Serial Number: 80-001207
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1012059 Exp: 09/05/2021
0.000	0.036 / 0.050	0.080	0.201	0.080
0.000	0.037 / 0.050	0.080	0.202	0.080
0.000	0.039 / 0.050	0.081	0.201	0.080

Number of Simulators Used: 5


Remarks:

LOOSE HOSE.

*Coupling on simulator hose was loose tightened
Coupling repaired test no issues.*

The above instrument complies (X) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

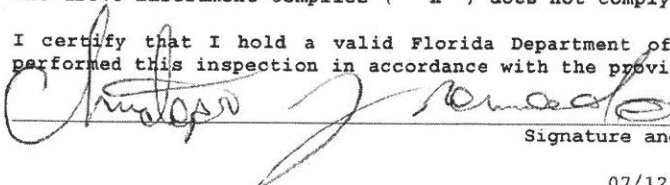

CHRISTOPHER J NORWOOD

Signature and Printed Name

07/12/2019
Date

1207
SP

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: HENDRY COUNTY S.O.
Time of Inspection: 00:56

Date of Inspection: 02/22/2019

Serial Number: 80-001207
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:437738 Exp: 06/08/2019
0.000	0.050	0.078	0.197	0.081
0.000	0.050	0.078	0.198	0.081
0.000	0.050	0.078	0.198	0.081


Number of Simulators Used: 5

Remarks:

A F / M A: Range Exceeded. *Used too much mouth alcohol. Test Repeated NO Issues.*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

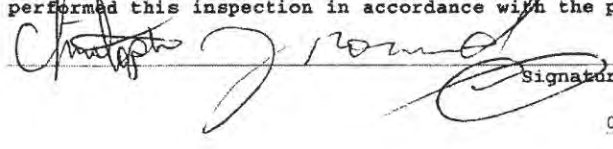

 Signature and Printed Name CHRISTOPHER J NORWOOD

 02/22/2019
 Date