

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 16:17

Date of Inspection: 12/30/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.052	0.077	0.196	0.080
0.000	0.052	0.078	0.197	0.080
0.000	0.052	0.078	0.196	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


DANIEL E LYONS

Signature and Printed Name

12/30/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
13K

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 13:37

Date of Inspection: 11/26/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.052	0.078	0.198	0.081
0.000	0.051	0.078	0.198	0.080
0.000	0.051	0.078	0.198	0.081

Number of Simulators Used: 4

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

11/26/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 22:06

Date of Inspection: 09/10/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.194	0.080
0.000	0.048	0.077	0.194	0.080
0.000	0.048	0.077	0.195	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

09/10/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 21:55

Date of Inspection: 08/02/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.077	0.197	0.080
0.000	0.048	0.077	0.199	0.080
0.000	0.048	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

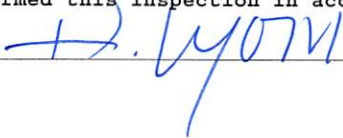

DANIEL E LYONS

Signature and Printed Name

08/02/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

7/3/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 23:37

Date of Inspection: 07/01/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.046	0.076	0.194	0.080
0.000	0.046	0.077	0.195	0.080
0.000	0.047	0.076	0.195	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D Lyons

DANIEL E LYONS

Signature and Printed Name

07/01/2019
Date



Florida Department of Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Osceola County SO

Instrument Serial Number: 80-001715

AGENCY INSPECTION DATA REVIEW		
Agency Inspector: Dan Lyons	Date of Inspection: 6/11/2019	Time of Inspection: 21:25
Agency Inspection Discrepancy: <input type="checkbox"/> Incomplete <input type="checkbox"/> Untimely/Not Received <input checked="" type="checkbox"/> Erroneous Information <input type="checkbox"/> Procedural <input type="checkbox"/> Other _____		
<input type="checkbox"/> Agency Inspection Not Conducted or Records regarding Agency Inspection have not been uploaded.		
<input checked="" type="checkbox"/> Lot Number <input type="checkbox"/> Expiration Date for <u>0.20g/ 210L</u> <input checked="" type="checkbox"/> Alcohol Reference Solution <input type="checkbox"/> Dry Gas Standard is <input checked="" type="checkbox"/> Incorrect <input type="checkbox"/> Expired.		
<input type="checkbox"/> FDLE/ATP Form 39 states in part, "If a test must be repeated, the REASON must be entered when prompted and recorded in the Remarks section of FDLE/ATP Form 40 Agency Inspection Report – Intoxilyzer 8000. The <input type="checkbox"/> REASON for repeating the following test(s); OR the <input type="checkbox"/> Possible Cause and Corrective Action Taken on the following test(s) was not recorded: <input type="checkbox"/> Alcohol Free Subject Test <input type="checkbox"/> Mouth Alcohol Test <input type="checkbox"/> Alcohol Free Test <input type="checkbox"/> Interferent Detect Test <input type="checkbox"/> 0.05 g/210L Test <input type="checkbox"/> 0.08 g/210L Test <input type="checkbox"/> 0.20 g/210L Test <input type="checkbox"/> 0.08 g/210L Dry Gas Standard Test		
<input type="checkbox"/> FDLE/ATP Form 39 states in part, "If the instrument does not comply with the requirements of Chapter 11D-8, FAC, remove the instrument from service and notify the Department Inspector." <input type="checkbox"/> The Department Inspector was not notified. However, the issue was satisfactorily corrected and the repeated Agency Inspection complies with the requirements of Chapter 11D-8, FAC. <input type="checkbox"/> The Department Inspector was not notified. However, the repeated Agency Inspection does not comply with the requirements of Chapter 11D-8, FAC and the instrument was correctly removed from evidentiary use. <input type="checkbox"/> The Department Inspector was not notified. The repeated Agency Inspection does not comply with the requirements of Chapter 11D-8, FAC and the instrument was not removed from evidentiary use.		
<input type="checkbox"/> The Agency Inspection is noted as "Complies" when it does not comply with the requirements of Chapter 11D-8, FAC.		
<input type="checkbox"/> Other: _____		

OTHER ELECTRONIC DATA REVIEW	
<input type="checkbox"/> Login Records Date: _____	Comments: The lot number for the 0.20 solution is incorrect. I suspect a typo, but I need the Agency Inspector of record to confirm. Please amend the form 40 and resubmit with the correct lot number.
<input type="checkbox"/> Cylinder Change Records Date: _____	
<input type="checkbox"/> Control Test Records Date: _____	
<input type="checkbox"/> Diagnostic Check Records Date: _____	

CORRECTIVE ACTION
<input checked="" type="checkbox"/> Record hand-written amendments on the FDLE/ATP Form 40, Agency Inspection Report, initial and date the amendments, mark the report "AMENDED", and forward a copy to the Department Inspector by <u>6/30/2019</u> (Date).
<input type="checkbox"/> Provide a written explanation regarding the referenced item(s) to the Department Inspector by _____ (Date).
<input type="checkbox"/> Upload the Agency Inspection(s).
<input type="checkbox"/> Remove the instrument from evidentiary use until otherwise directed by the Department.
<input type="checkbox"/> No action required
<input type="checkbox"/> Other: _____


Signature of Alcohol Testing Program Staff Member

6/13/2019
Date

Graham, Thomas

From: Dan Lyons <dlyo@OSCEOLA.ORG>
Sent: Monday, June 17, 2019 5:16 PM
To: Graham, Thomas; 'McKnight, Jamie (JMcknight@sao9.org)'; 'Atkinson, Karsona'; 'SherryForcier@flhsmv.gov'
Subject: Monthly Intox inspections for June
Attachments: 11 June 2019 Monthly Intox Inspec C.pdf

Follow Up Flag: FollowUp
Flag Status: Completed

ALCON,

I had an typo to correct on the report.

Instrument 80-001715, 0.20g/210L Test. I entered the Lot # as 021802G, it should be 201802G. See the correction made and attached.

Thank you

V/R

Dan Lyons
Osceola County Sheriff's Office
Spec Ops/Traffic/DUI Enforcement Unit
Agency 407-348-1100
Agency Cell 407-269-1980
Cell 321-960-2066

From: Dan Lyons
Sent: Thursday, June 13, 2019 1:25 AM
To: 'Graham, Thomas' <ThomasGraham@fdle.state.fl.us>; 'McKnight, Jamie (JMcknight@sao9.org)' <JMcknight@sao9.org>; 'Atkinson, Karsona' <KarsonaAtkinson@flhsmv.gov>; 'SherryForcier@flhsmv.gov' <SherryForcier@flhsmv.gov>
Cc: George Maroney <gmar2@OSCEOLA.ORG>
Subject: Monthly Intox inspections for June

ALCON,

Agency Inspection Report conducted 06/11/2019 on the following instruments;
80-000966, 80-000968, 80-001715, 80-003935, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-000966, I received an Temperature Regulation Test Fail during the Diagnostic test. I conducted a second check to confirm the same result. I removed the instrument from service and it will be forwarded to FDLE in the morning for evaluation and repairs.

Ref to instrument 80-003937, 0.08g/210L Test, received an outside control tolerance reading. I confirmed the simulator temperature and tighten the lid to the simulator and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-004587, 0.08g/210L Test, received an outside control tolerance reading for AF/MA. Provided MA breath showed a breath result. Rinsed mouth alcohol and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to the 0.08g/210L Dry Gas Std Test, received an outside control tolerance reading. I failed to connect the dry gas hose prior to starting the test. I connected the hose and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-005935, the 0.08g/210L Dry Gas Std Test, received an outside control tolerance reading. I failed to connect the dry gas hose prior to starting the test. I connected the hose and re-tested. The re-test results are with in standards. The inspection was not Re-Started

All intox inspections are complete and in compliance with 11D-8.

V/R

Dan Lyons
Osceola County Sheriff's Office
Spec Ops/Traffic/DUI Enforcement Unit
Agency 407-348-1100
Agency Cell 407-269-1980
Cell 321-960-2066

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 21:25

Date of Inspection: 06/11/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:021802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.193	0.080
0.000	0.047	0.076	0.194	0.080
0.000	0.047	0.076	0.194	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

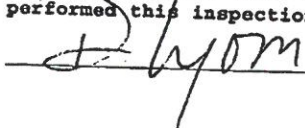

DANIEL E LYONS
Signature and Printed Name

06/11/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 21:25

Date of Inspection: 06/11/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.193	0.080
0.000	0.047	0.076	0.194	0.080
0.000	0.047	0.076	0.194	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

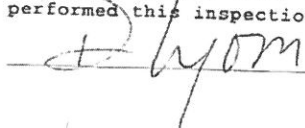

Signature and Printed Name DANIEL E LYONS

06/11/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

5/17/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 16:23

Date of Inspection: 05/15/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#: 201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 646645 Exp: 12/05/2019
0.000	0.048	0.076	0.194	0.079
0.000	0.049	0.077	0.196	0.080
0.000	0.048	0.077	0.198	0.080


Number of Simulators Used: 5

Remarks:

AF/MA. TOO MUCH MOUTH ALCO, ANOTHER DS PROVIDE AF RETESTED

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


DANIEL E LYONS

 Signature and Printed Name

05/15/2019
 Date

Graham, Thomas

From: Dan Lyons <dlyo@OSCEOLA.ORG>
Sent: Wednesday, May 15, 2019 7:47 PM
To: Graham, Thomas; 'Atkinson, Karsona'; 'McKnight, Jamie (JMcknight@sao9.org)'; 'SherryForcier@flhsmv.gov'; George Maroney
Subject: Monthly Intox Inspections May 2019
Attachments: 15 May 2019 Monthly Intox Inspec.pdf
Follow Up Flag: FollowUp
Flag Status: Flagged

80-001715
5/17/19
JA

ALCON,

Agency Inspection Report conducted 05/15/2019 due to the return of instrument 80-000966 from Annual Inspection. The report was conducted on the following instruments; 80-000966, 80-000968, 80-001715, 80-003935, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-001715, AF/MA, MA Alcohol test did not receive a Slope not met reading. The instrument was re-tested with AF provided by another Deputy. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-003935, AF/MA, MA Alcohol test did not receive a Slope not met reading. The instrument was re-tested with AF provided by another Deputy. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-003937, prompt showed Alcohol Free Test, hit N in error, which ended the test. The inspection was re-started. The results is within standards.

Instrument 80-000966 was returned from Annual Inspection, repairs and is back in service.

All intox inspections are complete and in compliance with 11D-8.

V/R

Dan Lyons
Osceola County Sheriff's Office
Spec Ops/Traffic/DUI Enforcement Unit
Agency 407-348-1100
Agency Cell 407-269-1980
Cell 321-960-2066

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

Florida Department of Law Enforcement Alcohol Testing Program

5/3/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 03:45

Date of Inspection: 05/02/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.076	0.195	0.081
0.000	0.048	0.077	0.195	0.080
0.000	0.049	0.077	0.195	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyons

DANIEL E LYONS
Signature and Printed Name

05/02/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

4/8/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 20:41

Date of Inspection: 04/03/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.049	0.077	0.196	0.080
0.000	0.049	0.078	0.197	0.080
0.000	0.049	0.078	0.197	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyons

DANIEL E LYONS

Signature and Printed Name

04/03/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

3/19/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 22:33

Date of Inspection: 03/18/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.041 / 0.047	0.075	0.192	0.079
0.000	0.043 / 0.047	0.077	0.194	0.080
0.000	0.047 / 0.047	0.077	0.194	0.079


Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance. **RE-SECURED LID TO SIMULATOR, RE-TESTED**

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


 _____ DANIEL E LYONS
 Signature and Printed Name

03/18/2019
 Date

Florida Department of Law Enforcement Alcohol Testing Program

2/15/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 19:19

Date of Inspection: 02/07/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.077	0.194	0.079
0.000	0.048	0.077	0.194	0.080
0.000	0.048	0.077	0.193	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

02/07/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

1/25/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 22:03

Date of Inspection: 01/24/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.195	0.080
0.000	0.048	0.077	0.195	0.080
0.000	0.047	0.077	0.192	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

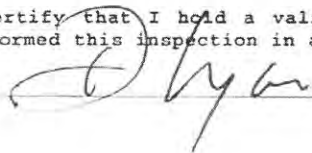

DANIEL E LYONS

Signature and Printed Name

01/24/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

1/7/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 00:38

Date of Inspection: 01/07/2019

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.045	0.075	0.193	0.080
0.000	0.046	0.077	0.198	0.080
0.000	0.046	0.078	0.198	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


 _____ DANIEL E LYONS
 Signature and Printed Name

01/07/2019
 Date