

Florida Department of Law Enforcement Alcohol Testing Program

80-004587
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 19:21

Date of Inspection: 12/30/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2020
0.000	0.051	0.075	0.191	0.076
0.000	0.052	0.076	0.197	0.077
0.000	0.053	0.077	0.197	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

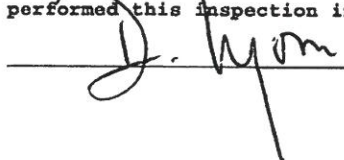

DANIEL E LYONS
Signature and Printed Name

12/30/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-4587
BLK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 14:36

Date of Inspection: 11/26/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.055	0.078	0.199	0.079
0.000	0.053	0.079	0.199	0.078
0.000	0.052	0.079	0.200	0.078

Number of Simulators Used: 4

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

11/26/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCROLA COUNTY S.O.
Time of Inspection: 23:54

Date of Inspection: 09/10/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.077	0.194	0.000 / 0.078
0.000	0.049	0.078	0.197	0.000 / 0.078
0.000	0.049	0.078	0.197	0.000 / 0.078

Number of Simulators Used: 5

Remarks:

08:Ctrl Outside Tolerance.DID NOT CONN DRY GAS TUBE/CONN/R

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



Signature and Printed Name DANIEL E LONS

09/10/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 20:35

Date of Inspection: 08/02/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.000 / 0.048	0.077	0.196	0.078
0.000	0.000 / 0.047	0.077	0.197	0.077
0.000	0.000 / 0.048	0.077	0.197	0.078


Number of Simulators Used: 5

Remarks:

05:Control Outside Tolerance/DID NOT CONNECT SIM/RE-TESTED . SIM CONNECTED/RE-TESTED/WITHIN STANDARD S

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

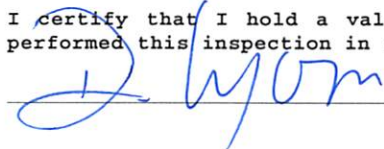

DANIEL E LYONS

Signature and Printed Name

08/02/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

7/3/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 01:21

Date of Inspection: 07/02/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.196	0.078
0.000	0.047	0.077	0.198	0.076
0.000	0.047	0.078	0.198	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


 _____ DANIEL E LYONS
 Signature and Printed Name

07/02/2019
 Date

Florida Department of Law Enforcement Alcohol Testing Program

6/13/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 00:59

Date of Inspection: 06/12/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#: 201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#: 201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 646645 Exp: 12/05/2019
0.000	0.047	0.076	0.195	0.000 / 0.078
0.000	0.047	0.077	0.197	0.000 / 0.077
0.000	0.047	0.077	0.197	0.000 / 0.077

Number of Simulators Used: 5

Remarks:

A F / M A: . 08: Control Outside Tolerance. **DID NOT CONNECT DRY GAS HOSE**
RINSED MOUTH
ALCOHOL / RE TESTED
HOSE CONNECTED / RETESTED

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D Lyons

DANIEL E LYONS

Signature and Printed Name

06/12/2019
Date

Graham, Thomas

From: Dan Lyons <dlyo@OSCEOLA.ORG>
Sent: Thursday, June 13, 2019 1:25 AM
To: Graham, Thomas; 'McKnight, Jamie (JMcknight@sao9.org)'; 'Atkinson, Karsona'; 'SherryForcier@flhsmv.gov'
Cc: George Maroney
Subject: Monthly Intox inspections for June
Attachments: 11 June 2019 Monthly Intox Inspec.pdf

Follow Up Flag: FollowUp
Flag Status: Flagged

80-004587
6/13/19
ja

ALCON,

Agency Inspection Report conducted 06/11/2019 on the following instruments;
80-000966, 80-000968, 80-001715, 80-003935, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-000966, I received an Temperature Regulation Test Fail during the Diagnostic test. I conducted a second check to confirm the same result. I removed the instrument from service and it will be forwarded to FDLE in the morning for evaluation and repairs.

Ref to instrument 80-003937, 0.08g/210L Test, received an outside control tolerance reading. I confirmed the simulator temperature and tighten the lid to the simulator and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-004587, 0.08g/210L Test, received an outside control tolerance reading for AF/MA. Provided MA breath showed a breath result. Rinsed mouth alcohol and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to the 0.08g/210L Dry Gas Std Test, received an outside control tolerance reading. I failed to connect the dry gas hose prior to starting the test. I connected the hose and re-tested. The re-test results are with in standards. The inspection was not Re-Started.

Ref to instrument 80-005935, the 0.08g/210L Dry Gas Std Test, received an outside control tolerance reading. I failed to connect the dry gas hose prior to starting the test. I connected the hose and re-tested. The re-test results are with in standards. The inspection was not Re-Started

All intox inspections are complete and in compliance with 11D-8.

V/R

Dan Lyons
Osceola County Sheriff's Office
Spec Ops/Traffic/DUI Enforcement Unit
Agency 407-348-1100
Agency Cell 407-269-1980
Cell 321-960-2066

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

Florida Department of Law Enforcement Alcohol Testing Program

5/17/19
JL

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 15:47

Date of Inspection: 05/15/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.046	0.077	0.197	0.077
0.000	0.047	0.078	0.198	0.076
0.000	0.047	0.077	0.199	0.077

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D Lyons

DANIEL E LYONS

Signature and Printed Name

05/15/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

5/3/19
20

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 04:01

Date of Inspection: 05/02/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.076	0.198	0.079
0.000	0.049	0.077	0.199	0.080
0.000	0.048	0.078	0.198	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D. Lyons

DANIEL E LYONS

Signature and Printed Name

05/02/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

4/8/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 20:23

Date of Inspection: 04/03/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.076	0.195	0.078
0.000	0.049	0.077	0.198	0.077
0.000	0.048	0.078	0.198	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS
Signature and Printed Name

04/03/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 19:43

Date of Inspection: 04/03/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.048	0.000 / 0.077		
0.000	0.049	0.078 / 0.079		
0.000	0.048	0.079 / 0.078		

Number of Simulators Used: 5

Remarks:

08:CNTRL OUT TOL SIM NOT HOOKED UP/HOOKED UP RETESTED.

*UPON COMPLETION OF RETEST (WITHIN STANDARDS) EXITED IN ERROR
INSTRUMENT RETESTED*

*4/8/19
JD*

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

D Lyons

Signature and Printed Name

DANIEL E LYONS

04/03/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

3/19/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 23:54

Date of Inspection: 03/18/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.049	0.077	0.197	0.078
0.000	0.049	0.078	0.198	0.077
0.000	0.050	0.078	0.197	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

03/18/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

2/15/19
JD

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.

Time of Inspection: 20:57

Date of Inspection: 02/07/2019

Serial Number: 80-004587

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.077	0.193	0.078
0.000	0.048	0.077	0.196	0.077
0.000	0.048	0.077	0.196	0.077


Number of Simulators Used: 5

Remarks:

AF/MA: Improper Sample PROVIDED/RETESTED

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS

Signature and Printed Name

02/07/2019

Date

Florida Department of Law Enforcement Alcohol Testing Program

1/25/19
JO

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 23:36

Date of Inspection: 01/24/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.047	0.076	0.194	0.077
0.000	0.047	0.077	0.196	0.078
0.000	0.047	0.076	0.196	0.076

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS
Signature and Printed Name

01/24/2019
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

1/7/19
JD

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 00:02

Date of Inspection: 01/07/2019

Serial Number: 80-004587
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	
	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201802B Exp: 02/06/2020	0.08g/210L Test (g/210L) Lot#:201709A Exp: 09/12/2019	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:646645 Exp: 12/05/2019
0.000	0.048	0.078	0.196	0.078
0.000	0.048	0.078	0.198	0.078
0.000	0.047	0.078	0.197	0.078

Number of Simulators Used: 5

Remarks:

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



DANIEL E LYONS
Signature and Printed Name

01/07/2019
Date