

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ST LUCIE COUNTY SO
Time of Inspection: 15:25

Date of Inspection: 01/31/2020

Serial Number: 80-000788
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	
		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:03519080A5 Exp: 04/05/2021
0.000	0.046	0.081	0.204	0.079
0.000	0.047	0.081	0.204	0.079
0.000	0.050	0.082	0.203	0.080

Number of Simulators Used: 5

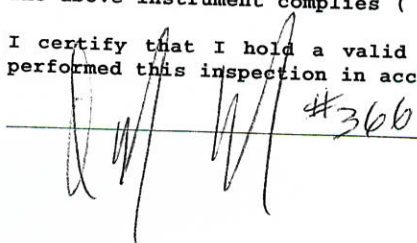
Remarks:

Non-compliance: .

DSP Test failed during diagnostic check.
~~Comms Transfer not connecting. Unable to upload.~~
 Comms Transfer uploaded 02/04/20

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 #366

Signature and Printed Name DAVID A CAGLIONI

01/31/2020
Date