

Florida Department of Law Enforcement Alcohol Testing Program

80-000968
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS
Time of Inspection: 14:09

Date of Inspection: 02/26/2020

Serial Number: 80-000968
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2020	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.049	0.076	0.195	0.080
0.000	0.049	0.077	0.196	0.079
0.000	0.048	0.077	0.194	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

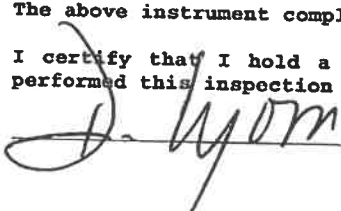

DANIEL E LYONS

Signature and Printed Name

02/26/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-000968
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS
Time of Inspection: 17:52

Date of Inspection: 02/07/2020

Serial Number: 80-000968
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.050	0.078	0.197	0.079
0.000	0.050	0.079	0.198	0.080
0.000	0.050	0.079	0.198	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

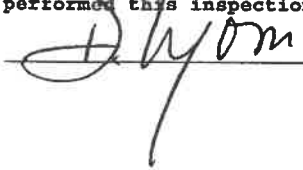

DANIEL E LYONS

Signature and Printed Name

02/07/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-000968
13K

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS
Time of Inspection: 14:49

Date of Inspection: 01/24/2020

Serial Number: 80-000968
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.050	0.077	0.194	0.080
0.000	0.050	0.077	0.195	0.080
0.000	0.050	0.077	0.195	0.080

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

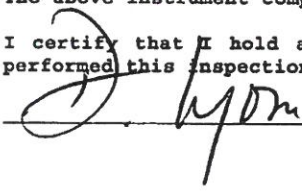

DANIEL E LYONS

Signature and Printed Name

01/24/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-000968
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA CORRECTIONS
Time of Inspection: 10:33

Date of Inspection: 01/03/2020

Serial Number: 80-000968
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1060911 Exp: 12/11/2021
0.000	0.051	0.076	0.195	0.079
0.000	0.050	0.077	0.195	0.079
0.000	0.050	0.077	0.194	0.079

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


DANIEL E LYONS

 Signature and Printed Name

01/03/2020
 Date