

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 14:54

Date of Inspection: 09/29/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201908B Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/02/2021	0.20g/210L Test (g/210L) Lot#: 201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: 32518080A2 Exp: 02/05/2021
0.000	0.048	0.078	0.198	0.075
0.000	0.049	0.079	0.199	0.076
0.000	0.049	0.079	0.199	0.075


Number of Simulators Used: 5

Remarks:

Time-Date changed.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

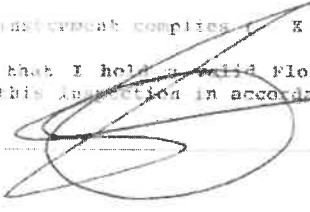

STEVE CASSEN
Signature and Printed Name

09/29/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 16:23

Date of Inspection: 08/26/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
/ 0.000	0.047	0.079	0.197	0.075
/ 0.000	0.048	0.081	0.197	0.075
/ 0.000	0.048	0.080	0.199	0.075

Number of Simulators Used: 5

Remarks:

00: Ambient Fail.OPEN ALCOHOL SAMPLE

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

08/26/2020
Date

TARPON SPRINGS PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001065
08/26/2020
Software: 8100.27

| WET CONTROL TEST |

Test	g/210L	Time
Air Blank	0.000	15:38
Control Test	0.082	15:38
Air Blank	0.000	15:39



Operator's Signature

TARPON SPRINGS PD
Intoxilyzer - Alcohol Analyzer
Model 8000 SN 80-001065
08/26/2020
Software: 8100.27

WET CONTROL TEST

Test	g/210L	Time
Air Blank	0.000	15:36
Control Test	0.049	15:36
Air Blank	0.000	15:37



Operator's Signature

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 10:04

Date of Inspection: 08/26/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:2019100 Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:_____ Exp:_____	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:_____ Exp:_____
0.000	0.049	0.071 / 0.074		
0.000	0.049	0.072 / 0.080		
0.000	0.049	0.075 / 0.080		

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance LOOSE GASKET ON SIM, Control . LOOSE GASKET REPLACEDNon-compliance:CON
TROL OUTSIDE TOLERANCE, BAD GASKET ON SIM.

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

08/26/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

Amended

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: EARPON SPRINGS PD
Time of Inspection: 14:47

Date of Inspection: 08/10/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.049	0.072 / 0.076	0.193	0.078
0.000	0.048	0.075 / 0.076	0.195	0.079
0.000	0.049	0.075 / 0.076	0.197	0.078

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance.

Amendment:
09-16-2020 Gasket on 0.08g/210L was replaced.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

[Signature]

STEVE GASSEN

Signature and Printed Name

08/10/2020
Date



Florida Department of
Law Enforcement

AGENCY INSPECTION AND OTHER ELECTRONIC DATA REVIEW

Agency: Tarpon Springs Police Department

Instrument Serial Number: 80-001065

AGENCY INSPECTION DATA REVIEW		
Agency Inspector: Steve Gassen	Date of Inspection: 08/10/2020	Time of Inspection: 14:47:48
Agency Inspection Discrepancy: <input type="checkbox"/> Incomplete <input type="checkbox"/> Untimely/Not Received <input type="checkbox"/> Erroneous Information <input type="checkbox"/> Procedural <input checked="" type="checkbox"/> Other (Missing Required Information)		
<input type="checkbox"/> Agency Inspection Not Conducted or Records regarding Agency Inspection have not been uploaded.		
<input type="checkbox"/> Lot Number <input type="checkbox"/> Expiration Date for ____g/ 210L <input type="checkbox"/> Alcohol Reference Solution <input type="checkbox"/> Dry Gas Standard is <input type="checkbox"/> Incorrect <input type="checkbox"/> Expired.		
<input checked="" type="checkbox"/> FDLE/ATP Form 39 states in part, "If a test must be repeated, the REASON must be entered when prompted and recorded in the Remarks section of FDLE/ATP Form 40 Agency Inspection Report – Intoxilyzer 8000. The <input checked="" type="checkbox"/> REASON for repeating the following test(s); OR the <input checked="" type="checkbox"/> Possible Cause and Corrective Action Taken on the following test(s) was not recorded: <input type="checkbox"/> Alcohol Free Subject Test <input type="checkbox"/> Mouth Alcohol Test <input type="checkbox"/> Alcohol Free Test <input type="checkbox"/> Interferent Detect Test <input type="checkbox"/> 0.05 g/210L Test <input checked="" type="checkbox"/> 0.08 g/210L Test <input type="checkbox"/> 0.20 g/210L Test <input type="checkbox"/> 0.08 g/210L Dry Gas Standard Test		
<input type="checkbox"/> FDLE/ATP Form 39 states in part, "If the instrument does not comply with the requirements of Chapter 11D-8, FAC, remove the instrument from service and notify the Department Inspector." <input type="checkbox"/> The Department Inspector was not notified. However, the issue was satisfactorily corrected and the repeated Agency Inspection complies with the requirements of Chapter 11D-8, FAC. <input type="checkbox"/> The Department Inspector was not notified. However, the repeated Agency Inspection does not comply with the requirements of Chapter 11D-8, FAC and the instrument was correctly removed from evidentiary use. <input type="checkbox"/> The Department Inspector was not notified. The repeated Agency Inspection does not comply with the requirements of Chapter 11D-8, FAC and the instrument was not removed from evidentiary use.		
<input type="checkbox"/> The Agency Inspection is noted as "Complies" when it does not comply with the requirements of Chapter 11D-8, FAC.		
<input type="checkbox"/> Other: _____		

OTHER ELECTRONIC DATA REVIEW	
<input type="checkbox"/> Login Records Date: _____	Comments: The 0.08 g/210 L Test was repeated. The reason for repeating the test, as well as the corrective action taken prior to repeating it, must be included. Please see below for the corrective action and return to your Department Inspector by 10/11/2020.
<input type="checkbox"/> Cylinder Change Records Date: _____	
<input type="checkbox"/> Control Test Records Date: _____	
<input type="checkbox"/> Diagnostic Check Records Date: _____	

CORRECTIVE ACTION
<input checked="" type="checkbox"/> Record hand-written amendments on the FDLE/ATP Form 40, Agency Inspection Report, initial and date the amendments, mark the report "AMENDED", and forward a copy to the Department Inspector by <u>10/11/2020</u> (Date).
<input type="checkbox"/> Provide a written explanation regarding the referenced item(s) to the Department Inspector by ____ (Date).
<input type="checkbox"/> Upload the Agency Inspection(s).
<input type="checkbox"/> Remove the instrument from evidentiary use until otherwise directed by the Department.
<input type="checkbox"/> No action required
<input type="checkbox"/> Other: _____

Taylor Gutshew

Signature of Alcohol Testing Program Staff Member

9/11/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 14:47

Date of Inspection: 08/10/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.049	0.072 / 0.076	0.193	0.078
0.000	0.048	0.075 / 0.076	0.195	0.079
0.000	0.049	0.075 / 0.076	0.197	0.078

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

08/10/2020
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 12:14

Date of Inspection: 07/31/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.048	0.077	0.184 / 0.192	0.078
0.000	0.047	0.077	0.187 / 0.195	0.077
0.000	0.048	0.078	0.188 / 0.195	0.077

Number of Simulators Used: 5

Remarks:

Time-Date changed. 20: Control Outside Tolerance.REPL GASKE

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

07/31/2020
Date

Florida Department of Law Enforcement

Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 12:14

Date of Inspection: 07/31/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted	Yes	
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.048	0.077	0.184 / 0.192	0.078
0.000	0.047	0.077	0.187 / 0.195	0.077
0.000	0.048	0.078	0.188 / 0.195	0.077


Number of Simulators Used: 5

Remarks:

Time-Date changed. 20: Control Outside Tolerance.REPL GASKE

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

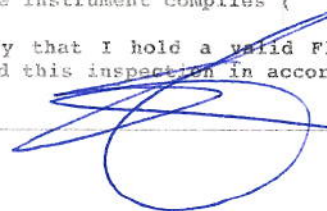

Signature and Printed Name

STEVE GASSEN

07/31/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD

Time of Inspection: 14:17

Date of Inspection: 06/29/2020

Serial Number: 80-001065

Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.046	0.077	0.197	0.077
0.000	0.046	0.078	0.199	0.078
0.000	0.047	0.078	0.198	0.077

Number of Simulators Used: 5

Remarks:

CLEANED AREA

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

STEVE GASSEN

Signature and Printed Name

06/29/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 15:28

Date of Inspection: 06/26/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#: 201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.044 / 0.045	0.077	0.197	
0.000	0.046 / 0.046	0.078	0.199	
0.000	0.045 / 0.046	0.077	0.200	


Number of Simulators Used: 5

Remarks:

05: Control Outside Tolerance LOOSE SEAL ON SIMULATOR. 20: RFI Detect CELL PHONE IN AREA WAS STILL 0 N, RFI Detect. Non-compliance: RFI DETECT TWICE.

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.



STEVE GASSEN

Signature and Printed Name

06/26/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 15:40

Date of Inspection: 05/29/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:32518080A2 Exp: 02/05/2021
0.000	0.047	0.078	0.197	0.078
0.000	0.050	0.078	0.198	0.077
0.000	0.051	0.078	0.200	0.078


Number of Simulators Used: 5

Remarks:

CLEANED AREA

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.


Signature and Printed Name

STEVE GASSEN

05/29/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-001065
YBK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: TARPON SPRINGS PD
Time of Inspection: 13:05

Date of Inspection: 02/27/2020

Serial Number: 80-001065
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 0019620 Exp: 02/28/2021	0.08g/210L Test (g/210L) Lot#: 0019620 Exp: 02/28/2021	0.20g/210L Test (g/210L) Lot#: 0019620 Exp: 02/28/2021	0.05 g/210L Dry Gas Std Test (g/210L) Lot#: 025180802 Exp: 02/05/2021
0.000	0.039 / 0.045	0.077	0.196	0.079
0.000	0.050 / 0.046	0.078	0.198	0.079
0.000	0.045 / 0.045	0.079	0.199	0.079

Source of Specimens Used: _____

Remarks:
One Breathalyzer found with loose battery on site.

The above instrument complies (☒) does not comply (☐) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

 STEVE GARSKE
Signature and Printed Name

02/27/2020
Date