

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.
Time of Inspection: 11:10

Date of Inspection: 09/08/2020

Serial Number: 80-001420
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.050	0.073 / 0.074		
0.000	0.050	0.073 / 0.075		
0.000	0.050	0.073 / 0.074		

Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance, Control Outside Tolerance. Non-compliance: USED DIFF. ARS ON REPEAT TESTING 201908B LOT, 08/07/2021 Expiration date. DI Platt notified via telephone on 09/08/2020 of non-compliance. *KM*

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

Kelly M Melville

Signature and Printed Name

09/08/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: ORANGE COUNTY S.O.
Time of Inspection: 11:10

Date of Inspection: 09/08/2020

Serial Number: 80-001420
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	
		No

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#: 201910D Exp: 10/22/2021	0.08g/210L Test (g/210L) Lot#: 201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#: Exp:	0.08 g/210L Dry Gas Std Test (g/210L) Lot#: Exp:
0.000	0.050	0.073 / 0.074		
0.000	0.050	0.073 / 0.075		
0.000	0.050	0.073 / 0.074		


Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance, Control Outside Tolerance. Non-compliance: USED DIFF. ARS ON REPEAT TESTING 201908B LOT, 08/07/2021 Expiration date. DI Platt notified via telephone on 09/08/2020 of non-compliance. *dm*

The above instrument complies () does not comply (X) with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

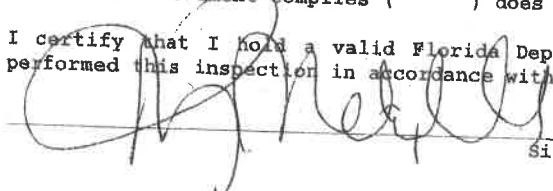

KELLY M MELVILLE
Signature and Printed Name

09/08/2020
Date