

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 14:54

Date of Inspection: 02/26/2020

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		
Diagnostic Check (Pre-Inspection): OK		No
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201908B Exp: 08/07/2021	0.20g/210L Test (g/210L) Lot#:201902C Exp: 02/20/2021	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.048	0.076	0.198	0.081
0.000	0.050	0.078	0.199	0.080
0.000	0.049	0.078	0.199	0.081

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

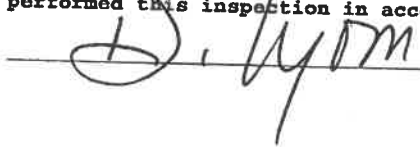

DANIEL E LYONS

Signature and Printed Name

02/26/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 17:40

Date of Inspection: 02/07/2020

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	


Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.051	0.078	0.196	0.083
0.000	0.051	0.077	0.197	0.083
0.000	0.051	0.078	0.197	0.082

Number of Simulators Used: 5

Remarks:

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

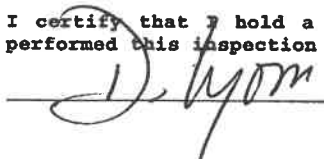

DANIEL E LYONS

Signature and Printed Name

02/07/2020
Date

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 14:26

Date of Inspection: 01/24/2020

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.051	0.195 / 0.077	0.195	0.081
0.000	0.051	0.197 / 0.077	0.196	0.081
0.000	0.051	0.196 / 0.077	0.196	0.081


Number of Simulators Used: 5

Remarks:

08: Control Outside Tolerance. ATTACHED 0.20 SIM ERROR / ATT CORRECT SIM / RETESTED

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

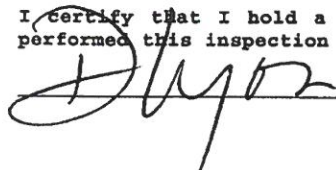

DANIEL E LYONS

Signature and Printed Name

01/24/2020
Date

Kirkland, Brett

From: Dan Lyons <dlyo@OSCEOLA.ORG>
Sent: Friday, January 24, 2020 7:07 PM
To: Platt, Shayla; 'McKnight, Jamie (JMcknight@sao9.org)'; 'SherryForcier@flhsmv.gov'; 'Atkinson, Karsona'; 'orlandobar@flhsmv.gov'; Brian Adams; Michael Hernandez
Cc: Alcohol Testing Program
Subject: RE: Jan 2020 Monthly Intox Inspections
Attachments: 24 Jan 2020 Monthly Intox Inspec.pdf

ALCON,

I received instrument 80-001715 back from the required Annual Inspection by FDLE on 01/23/2020. The inspection was completed on 01/16/2020.

The monthly Agency Inspection Report was conducted 01/024/2020 on the following instruments; 80-000966, 80-000968, 80-001715, 80-003937, 80-004587 and 80-005935.

Ref to instrument 80-001715, the 0.08g/210L Test. Received Outside Tolerance. I connected the simulator with the 0.20 solution. The instrument was re-tested with the simulator with the correct 0.08g solution, not re-started. The re-test results are within standards.

Ref to instrument 80-003935, it is still out at CMI for repair.

In reference to 80-000966, it has been sent out to FDLE for the annual inspection.

All intox inspections are complete and in compliance with 11D-8.

Thank you

V/R

Dan Lyons
Osceola County Sheriff's Office
Spec Ops/Traffic/DUI Enforcement Unit
Agency 407-348-1100
Agency Cell 407-269-1980
Cell 321-960-2066

Attention: The information contained in this E-mail message is privileged and confidential information intended only for the use of the individual(s) named above. If the reader of this message is not the intended recipient, you are hereby notified that any dissemination, distribution or copy of this communication is strictly prohibited. If you have received this communication in error, please contact the sender by reply E-mail and destroy all copies of the original message.

Florida Department of Law Enforcement Alcohol Testing Program

80-001715
BK

AGENCY INSPECTION REPORT - INTOXILYZER 8000

Agency: OSCEOLA COUNTY S.O.
Time of Inspection: 10:34

Date of Inspection: 01/03/2020

Serial Number: 80-001715
Software: 8100.27

Check or Test	YES	NO
Date and/or Time Adjusted		No
Diagnostic Check (Pre-Inspection): OK	Yes	
Alcohol Free Subject Test: 0.000	Yes	
Mouth Alcohol Test: Slope Not Met	Yes	
Interferent Detect Test: Interferent Detect	Yes	
Diagnostic Check (Post-Inspection): OK	Yes	

Alcohol Free Test (g/210L)	0.05g/210L Test (g/210L) Lot#:201811C Exp: 11/13/2020	0.08g/210L Test (g/210L) Lot#:201808E Exp: 08/22/2020	0.20g/210L Test (g/210L) Lot#:201802G Exp: 02/22/2020	0.08 g/210L Dry Gas Std Test (g/210L) Lot#:1190213 Exp: 08/28/2022
0.000	0.052	0.075	0.186 / 0.195	0.082
0.000	0.052	0.076	0.191 / 0.196	0.082
0.000	0.051	0.076	0.193 / 0.196	0.082


Number of Simulators Used: 5

Remarks:

20: Control Outside Tolerance, RESET LID/CONNECTIONS. *RE-TESTED*

The above instrument complies () does not comply () with Chapter 11D-8, FAC.

I certify that I hold a valid Florida Department of Law Enforcement Agency Inspector Permit and that I performed this inspection in accordance with the provisions of Chapter 11D-8, FAC.

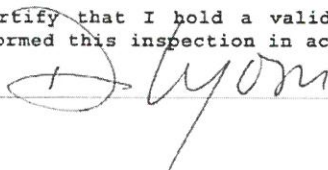

DANIEL E LYONS

Signature and Printed Name

01/03/2020
Date